

December 2014

artus[®] VZV RG PCR Kit Handbook



24 (catalog no. 4502263)



96 (catalog no. 4502265)

Version 1

IVD

Quantitative in vitro diagnostics

For use with Rotor-Gene[®] Q Instruments



REF

4502263, 4502265



1056824EN



QIAGEN GmbH, QIAGEN Strasse 1, 40724 Hilden, GERMANY

R4

MAT

1056824EN



Sample & Assay Technologies

QIAGEN Sample and Assay Technologies

QIAGEN is the leading provider of innovative sample and assay technologies, enabling the isolation and detection of contents of any biological sample. Our advanced, high-quality products and services ensure success from sample to result.

QIAGEN sets standards in:

- Purification of DNA, RNA, and proteins
- Nucleic acid and protein assays
- microRNA research and RNAi
- Automation of sample and assay technologies

Our mission is to enable you to achieve outstanding success and breakthroughs. For more information, visit www.qiagen.com.

Contents

Intended Use	4
Summary and Explanation	4
Pathogen information	4
Principle of the Procedure	4
Materials Provided	5
Kit contents	5
Materials Required but Not Provided	6
Warnings and Precautions	6
General precautions	7
Reagent Storage and Handling	7
Procedure	8
DNA isolation	8
Internal control	8
Protocol	
■ PCR and data analysis	9
Interpretation of Results	16
Quantitation	16
Results	17
Troubleshooting guide	18
Quality Control	20
Limitations	20
Performance Characteristics	21
Analytical sensitivity	21
Specificity	21
Precision	23
References	25
Symbols	25
Contact Information	26
Ordering Information	27

Intended Use

The *artus* VZV RG PCR Kit is an in vitro nucleic acid amplification test for the quantitation of VZV DNA in human cerebral spinal fluid (CSF). This diagnostic test kit utilizes the polymerase chain reaction (PCR) and is configured for use with Rotor-Gene Q Instruments.

Note: The *artus* VZV RG PCR Kit may not be used with Rotor-Gene Q 2plex Instruments.

Summary and Explanation

The *artus* VZV RG PCR Kit constitutes a ready-to-use system for the detection of VZV DNA using polymerase chain reaction (PCR) on Rotor-Gene Q Instruments. The VZV RG Master contains reagents and enzymes for the specific amplification of an 82 bp region of the VZV genome, and for the direct detection of the specific amplicon in fluorescence channel Cycling Green of the Rotor-Gene Q MDx, Rotor-Gene Q, or Rotor-Gene 6000 (source 470 nm, detector 510 nm).

In addition, the *artus* VZV RG PCR Kit contains a second heterologous amplification system to identify possible PCR inhibition. This is detected as an internal control (IC) in fluorescence channel Cycling Orange of the Rotor-Gene Q, or Rotor-Gene 6000 (source 585 nm, detector 610 nm). The detection limit of the analytical VZV PCR (see “Analytical sensitivity”, page 21) is not reduced. External positive controls (VZV RG QS 1–4) are supplied, which allow the determination of the amount of viral DNA. For further information, see “Quantitation”, page 16.

Pathogen information

The varicella-zoster virus (VZV) is a DNA virus, which is transmitted from person to person as a droplet infection or by direct contact. Infection with VZV causes slightly raised temperatures and affects the general health to a moderate extent. Polymorphic exema with welts, blisters, and scabs along with severe itching (chicken pox) are characteristic of the illness. Severe VZV infections are frequently observed with immunosuppressed patients and can result in dangerous complications, such as pneumonia and encephalitis. After the acute infection, the pathogen persists in the sensory spinal ganglia and in the ganglia of the cranial nerves. If immunity is weakened, exacerbations can occur (e.g., shingles).

Principle of the Procedure

Pathogen detection by the polymerase chain reaction (PCR) is based on the amplification of specific regions of the pathogen genome. In real-time PCR the

amplified product is detected via fluorescent dyes. These are usually linked to oligonucleotide probes that bind specifically to the amplified product. Monitoring the fluorescence intensities during the PCR run (i.e., in real-time) allows the detection and quantitation of the accumulating product without having to re-open the reaction tubes after the PCR run.*

Materials Provided

Kit contents

artus VZV RG PCR Kit			(24)	(96)
Catalog no.			4502263	4502265
Number of reactions			24	96
Blue	VZV RG Master		2 x 12 reactions	8 x 12 reactions
Yellow	VZV RG Mg-Sol [†]	Mg-Sol	600 µl	600 µl
Red	VZV RG QS 1 [‡] (1 x 10 ⁴ copies/µl)	QS	200 µl	200 µl
Red	VZV RG QS 2 [‡] (1 x 10 ³ copies/µl)	QS	200 µl	200 µl
Red	VZV RG QS 3 [‡] (1 x 10 ² copies/µl)	QS	200 µl	200 µl
Red	VZV RG QS 4 [‡] (1 x 10 ¹ copies/µl)	QS	200 µl	200 µl
Green	VZV RG IC [§]	IC	1000 µl	2 x 1000 µl
White	Water (PCR grade)		1000 µl	1000 µl
	Handbook		1	1

[†] Magnesium solution.

[‡] Quantitation standard.

[§] Internal control.

* Mackay, I.M. (2004) Real-time PCR in the microbiology laboratory. Clin. Microbiol. Infect. **10**, 190.

Materials Required but Not Provided

When working with chemicals, always wear a suitable lab coat, disposable gloves, and protective goggles. For more information, consult the appropriate safety data sheets (SDSs), available from the product supplier.

Reagents

- DNA isolation kit (see “DNA isolation”, page 8)

Consumables

- Sterile pipet tips with filters
- Strip Tubes and Caps, 0.1 ml, for use with 72-well rotor (cat. no. 981103 or 981106)
- Alternatively: PCR Tubes, 0.2 ml, for use with 36-well rotor (cat. no. 981005 or 981008)

Equipment

- Pipets (adjustable)*
- Vortex mixer*
- Benchtop centrifuge* with rotor for 2 ml reaction tubes
- Rotor-Gene Q MDx, Rotor-Gene Q, or Rotor-Gene Instrument*[†] with fluorescence channels for Cycling Green and Cycling Orange
- Rotor-Gene Q MDx/Rotor-Gene Q software version 1.7.94 or higher (Rotor-Gene 6000 software version 1.7.65, 1.7.87, 1.7.94)
- Cooling block (Loading Block 72 x 0.1 ml Tubes, cat. no. 9018901, or Loading Block 96 x 0.2 ml Tubes, cat. no. 9018905)

Warnings and Precautions

For in vitro diagnostic use

When working with chemicals, always wear a suitable lab coat, disposable gloves, and protective goggles. For more information, please consult the appropriate safety data sheets (SDSs). These are available online in convenient and compact PDF format at www.qiagen.com/safety where you can find, view, and print the SDS for each QIAGEN[®] kit and kit component.

Discard sample and assay waste according to your local safety regulations.

* Ensure that instruments have been checked and calibrated according to the manufacturer's recommendations.

[†] The *artus* VZV RG PCR Kit may not be used with Rotor-Gene Q 2plex Instruments.

General precautions

The user should always pay attention to the following:

- Use sterile pipet tips with filters.
- Store and extract positive materials (specimens, positive controls, and amplicons) separately from all other reagents, and add them to the reaction mix in a spatially separated facility.
- Thaw all components thoroughly at room temperature (15–25°C) before starting an assay.
- When thawed, mix the components (by pipetting repeatedly up and down or by pulse vortexing) and centrifuge briefly.
- Work quickly and keep components on ice or in the cooling block (72/96-well loading block).

Reagent Storage and Handling

The components of the *artus* VZV RG PCR Kit should be stored at –15°C to –30°C and are stable until the expiration date stated on the label. Repeated thawing and freezing (>2 x) should be avoided, as this may reduce assay sensitivity. If the reagents are to be used only intermittently, they should be frozen in aliquots. Storage at 2–8°C should not exceed a period of 5 hours.

Procedure

DNA isolation

The EZ1 DSP Virus Kit (QIAGEN, cat. no. 62724)* is validated for viral nucleic acid purification from human CSF, for use with the *artus* VZV RG PCR Kit. Carry out the viral nucleic acid purification according to the instructions in the *EZ1 DSP Virus Kit Handbook*, with a starting sample size of 200 μ l.

Note: The *artus* VZV RG PCR Kit should not be used with phenol-based isolation methods.

Note: The use of carrier RNA is critical for extraction efficiency and, consequently, for DNA/RNA yield. Add the appropriate amount of carrier RNA to each extraction following the instructions in the *EZ1 DSP Virus Kit Handbook*.

Note: The internal control of the *artus* VZV RG PCR Kit can be used directly in the isolation procedure (see "Internal control", below).

Internal control

An internal control (VZV RG IC) is supplied. This allows the user both to control the DNA isolation procedure and to check for possible PCR inhibition. For this application, add the internal control to the isolation at a ratio of 0.1 μ l per 1 μ l elution volume. For example, using the EZ1 DSP Virus Kit, if the viral nucleic acids are eluted in 60 μ l Elution Buffer (AVE), then 6 μ l of the internal control should be added initially.

Note: The internal control and carrier RNA (see "DNA isolation", page 8) should be added only to the mixture of lysis buffer and sample material or directly to the lysis buffer.

The internal control must not be added to the sample material directly. If added to the lysis buffer please note that the mixture of internal control and lysis buffer-carrier RNA has to be prepared freshly and used immediately (storage of the mixture at room temperature or in the fridge for only a few hours may lead to internal control failure and a reduced extraction efficiency).

Note: Do not add the internal control and the carrier RNA to the sample material directly.

The internal control can optionally be used exclusively to check for possible PCR inhibition. For this application, add the internal control directly to the mixture of VZV RG Master and VZV RG Mg-Sol, as described in step 2b of the protocol (page 10).

* The EZ1 DSP Virus Kit is also available as CE-IVD-marked EASYartus® VZV RG PCR Kits, combined with the *artus* VZV RG PCR Kit (see page 27 for ordering information).

Protocol: PCR and data analysis

Important points before starting

- Take time to familiarize yourself with the Rotor-Gene Q Instrument before starting the protocol. See the instrument user manual.
- Make sure that at least one quantitation standard as well as one negative control (Water, PCR grade) are included per PCR run. To generate a standard curve, use all 4 quantitation standards supplied (VZV RG QS 1–4) for each PCR run.

Things to do before starting

- Make sure that the cooling block (accessory of the Rotor-Gene Q Instrument) is precooled to 2–8°C.
- Before each use, all reagents need to be thawed completely, mixed (by repeated up and down pipetting or by quick vortexing), and centrifuged briefly.

Procedure

- 1. Place the desired number of PCR tubes into the adapters of the cooling block.**
- 2. If you are using the internal control to monitor the DNA isolation procedure and to check for possible PCR inhibition, follow step 2a. If you are using the internal control exclusively to check for PCR inhibition, follow step 2b.**
 - 2a. The internal control has already been added to the isolation (see “Internal control”, page 8). In this case, prepare a master mix according to Table 1.**

The reaction mix typically contains all of the components needed for PCR except the sample.

Table 1. Preparation of master mix (internal control used to monitor DNA isolation and check for PCR inhibition)

Number of samples	1	12
VZV RG Master	25.5 μ l	306 μ l
VZV RG Mg-Sol	4.5 μ l	54 μ l
VZV RG IC	0 μ l	0 μ l
Total volume	30 μl	360 μl

- 2b. The internal control must be added directly to the mixture of VZV RG Master and VZV RG Mg-Sol. In this case, prepare a master mix according to Table 2.**

The reaction mix typically contains all of the components needed for PCR except the sample.

Table 2. Preparation of master mix (internal control used exclusively to check for PCR inhibition)

Number of samples	1	12
VZV RG Master	25.5 μ l	306 μ l
VZV RG Mg-Sol	4.5 μ l	54 μ l
VZV RG IC	2 μ l	24 μ l
Total volume	32 μl*	384 μl*

* The volume increase caused by adding the internal control is neglected when preparing the PCR assay. The sensitivity of the detection system is not impaired.

- 3. Pipet 30 μ l of the master mix into each PCR tube. Then add 20 μ l of the eluted sample DNA (see Table 3). Correspondingly, 20 μ l of at least one of the quantitation standards (VZV RG QS 1–4) must be used as a positive control and 20 μ l of water (Water, PCR grade) as a negative control.**

Table 3. Preparation of PCR assay

Number of samples	1	12
Master mix	30 μ l	30 μ l each
Sample	20 μ l	20 μ l each
Total volume	50 μl	50 μl each

4. **Close the PCR tubes. Make sure that the locking ring (accessory of the Rotor-Gene Instrument) is placed on top of the rotor to prevent accidental opening of the tubes during the run.**
5. **For the detection of VZV DNA, create a temperature profile according to the following steps.**

Setting the general assay parameters	Figures 1, 2, 3
Initial activation of the hot-start enzyme	Figure 4
Amplification of the DNA	Figure 5
Adjusting the fluorescence channel sensitivity	Figure 6
Starting the run	Figure 7

All specifications refer to the Rotor-Gene Q MDx/Rotor-Gene Q software version 1.7.94 and Rotor-Gene 6000 software versions 1.7.65, 1.7.87, and 1.7.94. Please find further information on programming Rotor-Gene Instruments in the instrument user manual. In the illustrations these settings are framed in bold black. Illustrations are included for Rotor-Gene Q Instruments.

6. First, open the “New Run Wizard” dialog box (Figure 1). Check the “Locking Ring Attached” box and click “Next”.

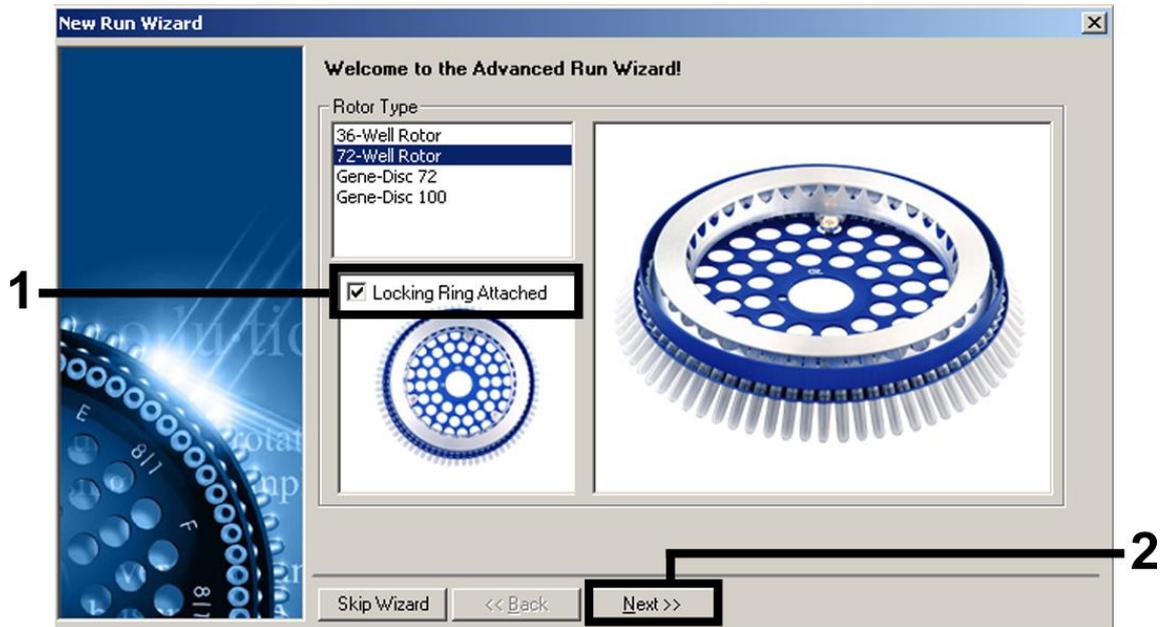


Figure 1. The “New Run Wizard” dialog box.

7. Select 50 for the PCR reaction volume and click “Next” (Figure 2).

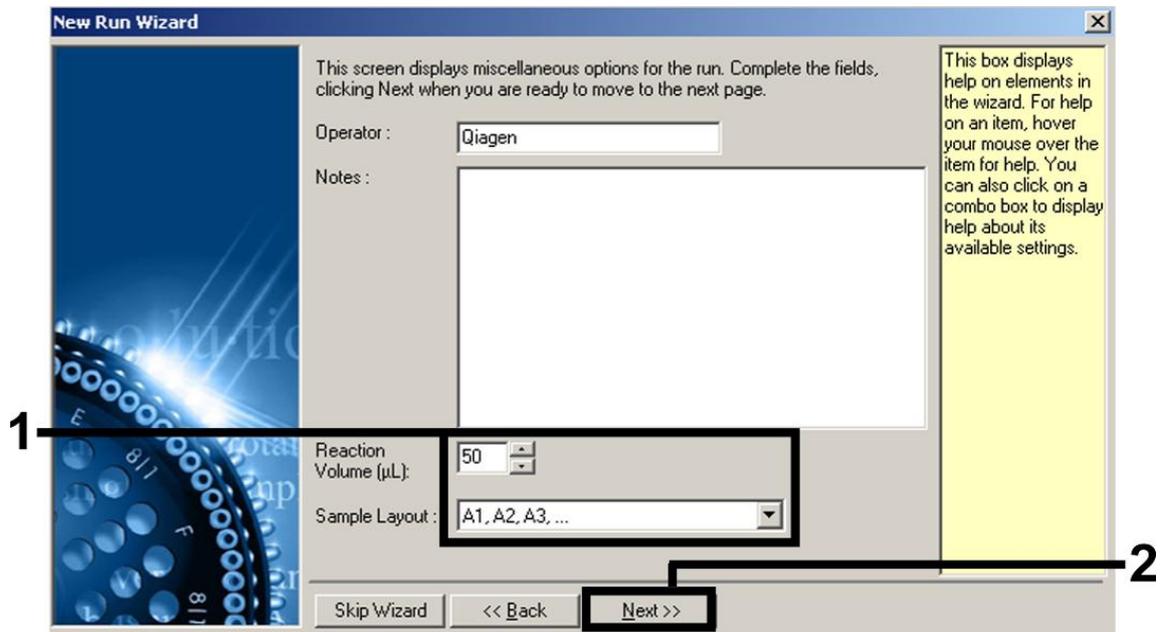


Figure 2. Setting the general assay parameters.

- Click the "Edit Profile" button in the next "New Run Wizard" dialog box (Figure 3), and program the temperature profile as shown in Figures 3–5).

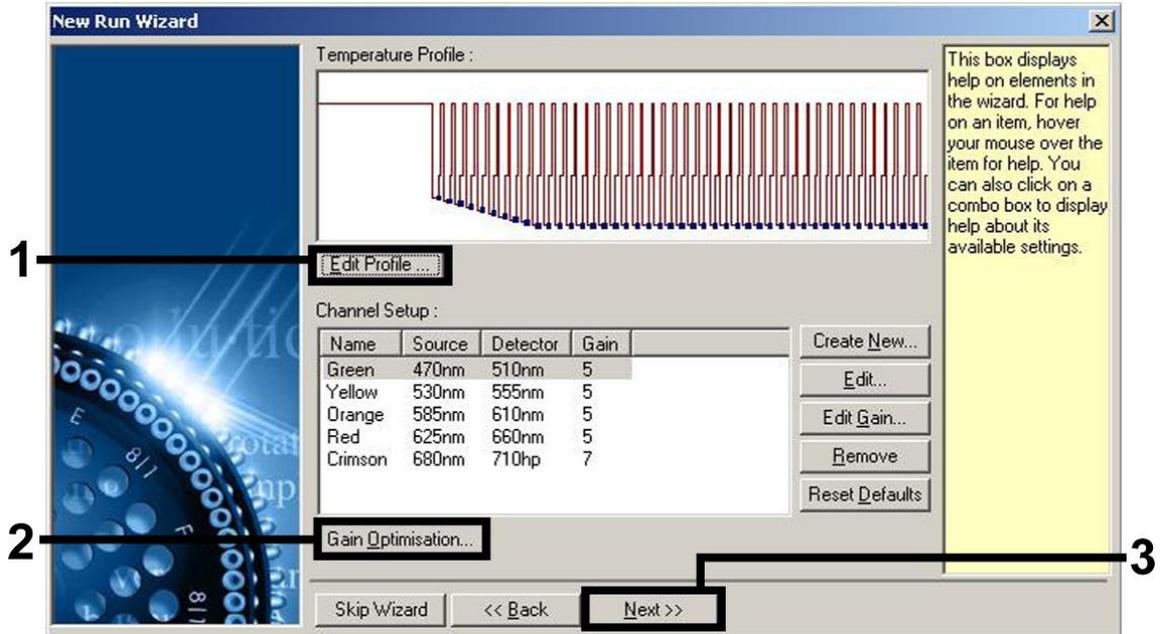


Figure 3. Editing the profile.

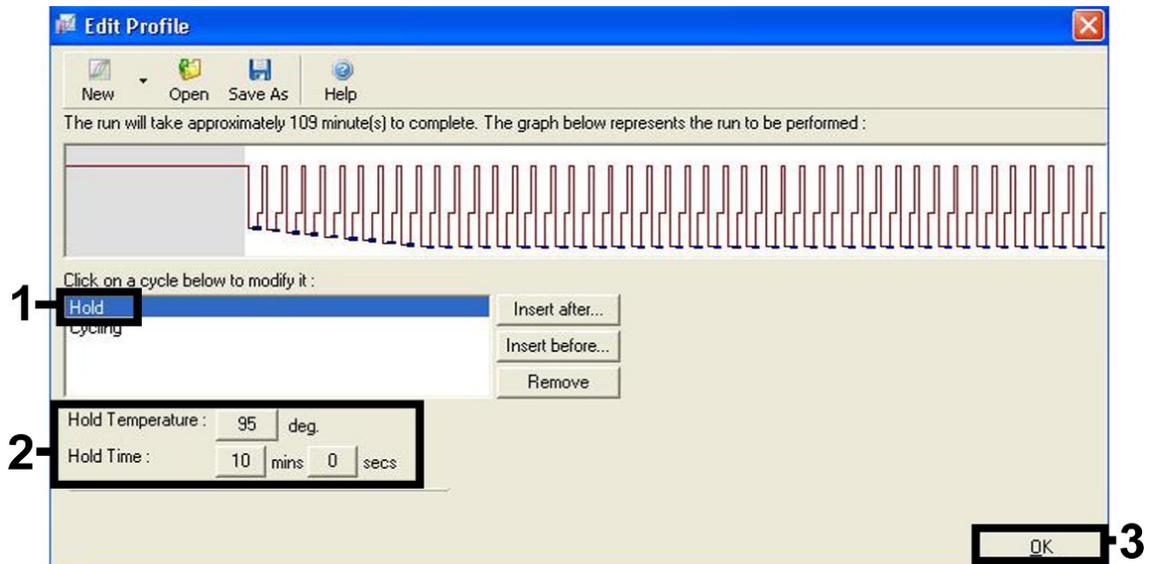


Figure 4. Initial activation of the hot-start enzyme.

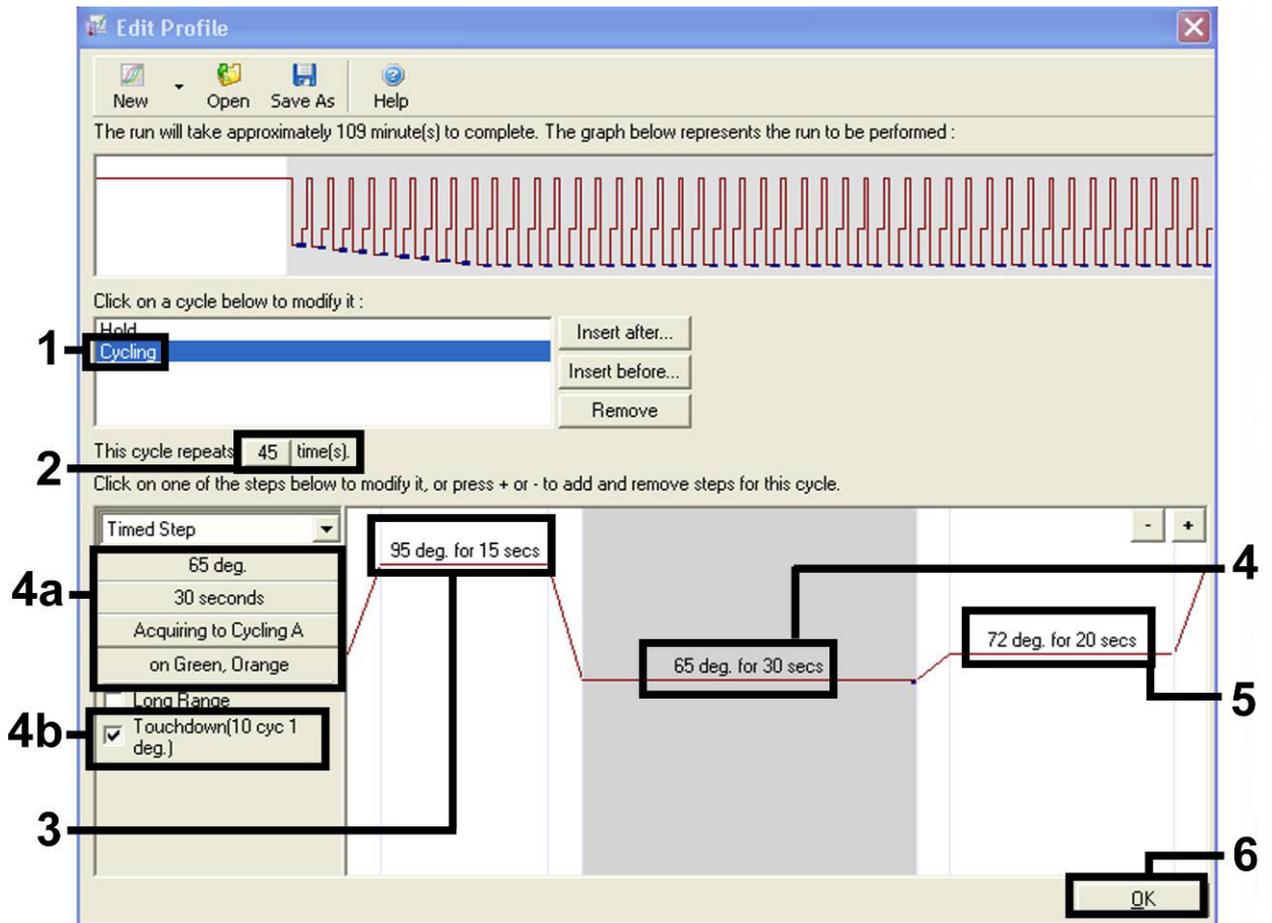


Figure 5. Amplification of the DNA. Make sure to activate the touchdown function for 10 cycles in the annealing step.

9. The detection range of the fluorescence channels has to be determined according to the fluorescence intensities in the PCR tubes. Click "Gain Optimisation" in the "New Run Wizard" dialog box (see Figure 3) to open the "Auto-Gain Optimisation Setup" dialog box. Set the calibration temperature to 65 to match the annealing temperature of the amplification program (Figure 6).

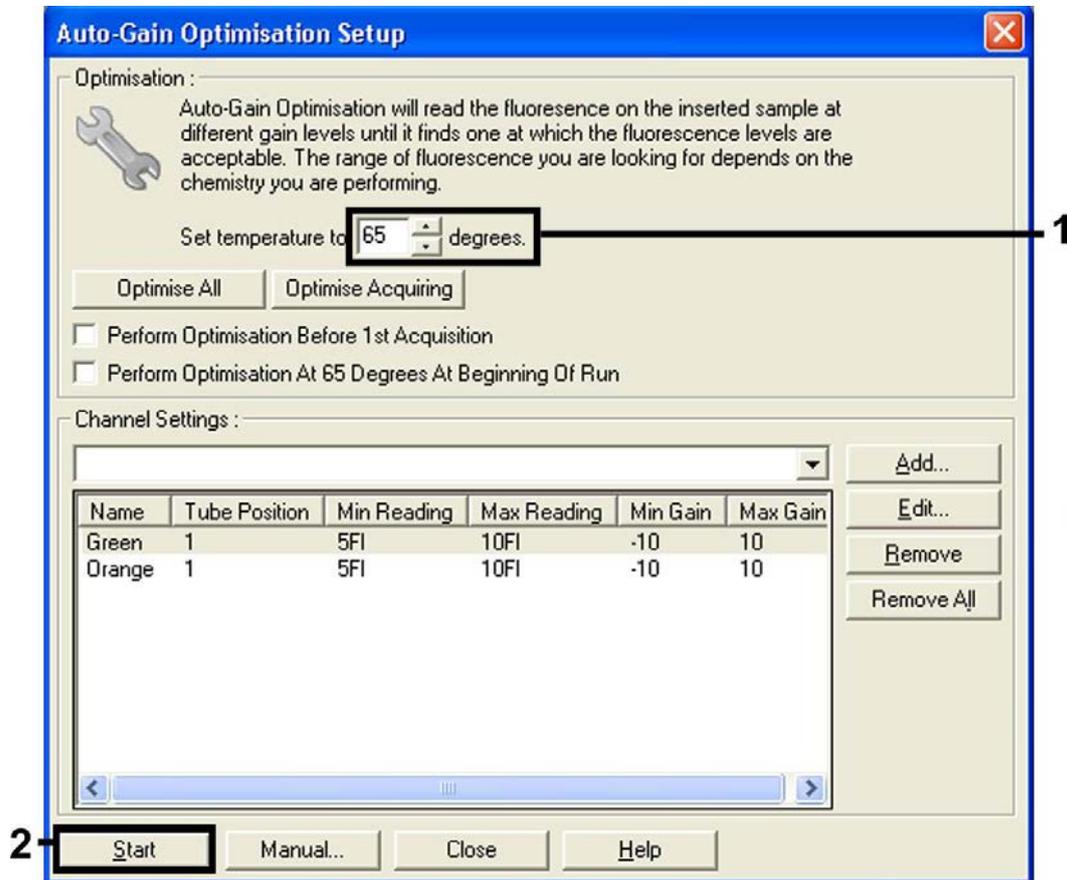


Figure 6. Adjusting the fluorescence channel sensitivity.

10. The gain values determined by the channel calibration are saved automatically and are listed in the last menu window of the programming procedure (Figure 7). Click “Start Run”.

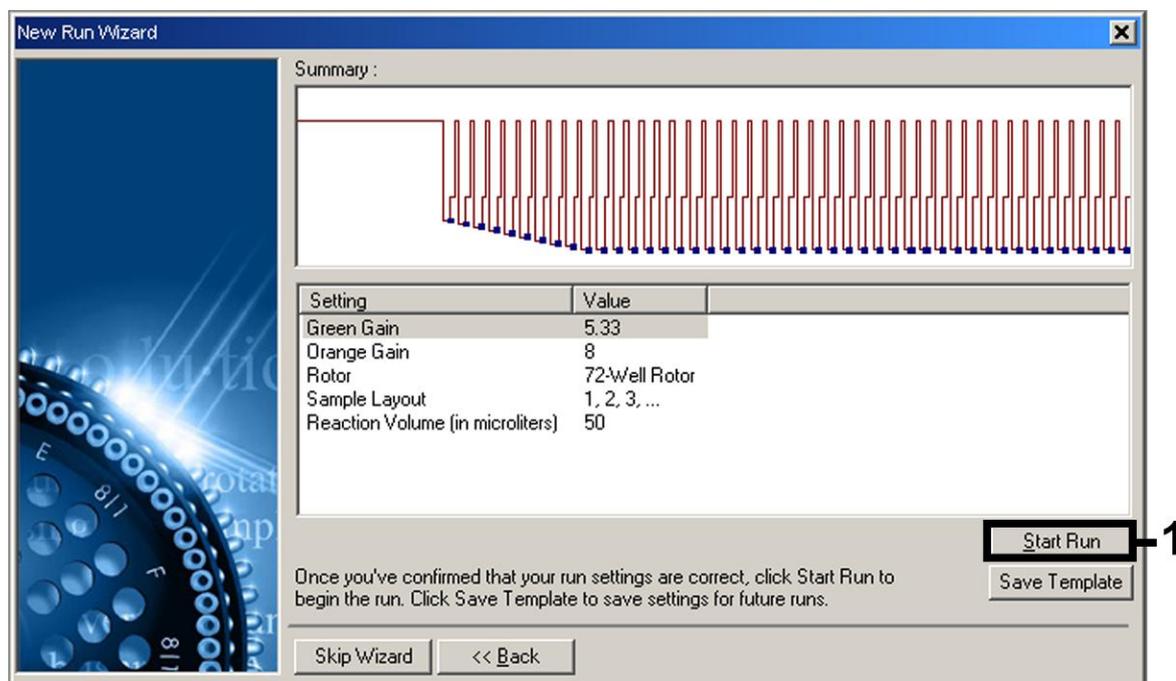


Figure 7. Starting the run.

Interpretation of Results

Quantitation

The enclosed quantitation standards (VZV RG QS 1–4) are treated as previously purified samples and the same volume is used (20 μ l). To generate a standard curve on Rotor-Gene Q Instruments, all 4 quantitation standards should be used and defined in the “Edit Samples” dialog box as standards with the specified concentrations (see the instrument user manual).

Note: The quantitation standards are defined as copies/ μ l. The following equation has to be applied to convert the values determined using the standard curve into copies/ml of sample material:

$$\text{Result (copies/ml)} = \frac{\text{Result (copies}/\mu\text{l)} \times \text{Elution Volume } (\mu\text{l})}{\text{Sample Volume (ml)}}$$

As a matter of principle the initial sample volume should be entered in the equation above. This has to be considered when the sample volume has been changed prior to the nucleic acid extraction (e.g., reducing the volume by centrifugation or increasing the volume by adding to the volume required for the isolation).

Results

Examples of positive and negative PCR reactions are given in Figure 8 and Figure 9.

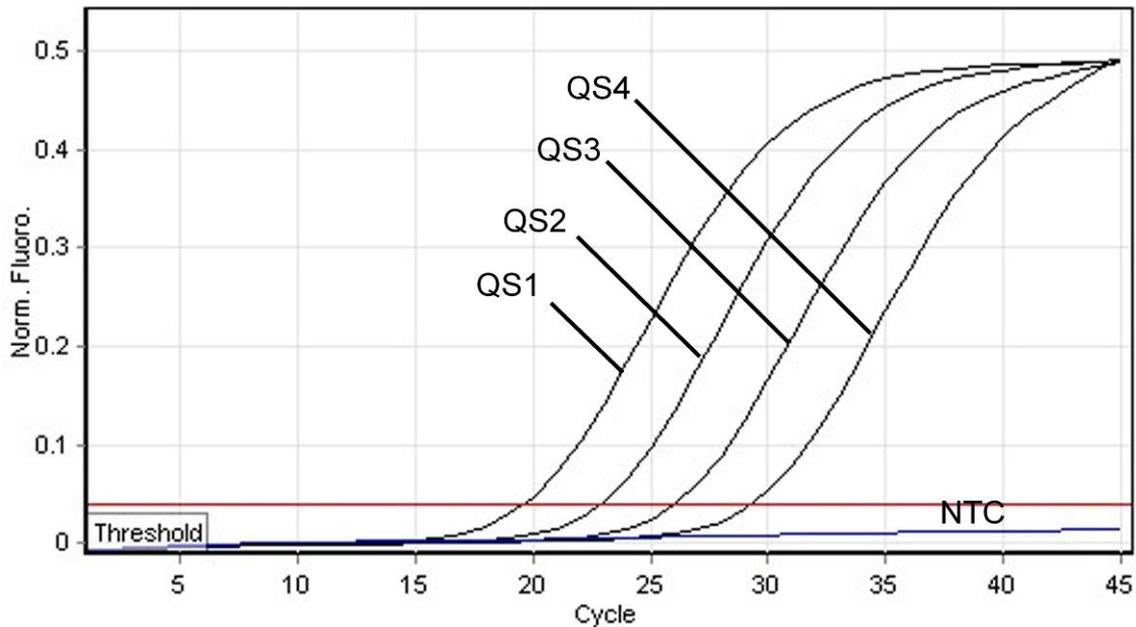


Figure 8. Detection of the quantitation standards (VZV RG QS 1–4) in fluorescence channel Cycling Green. NTC: No template control (negative control).

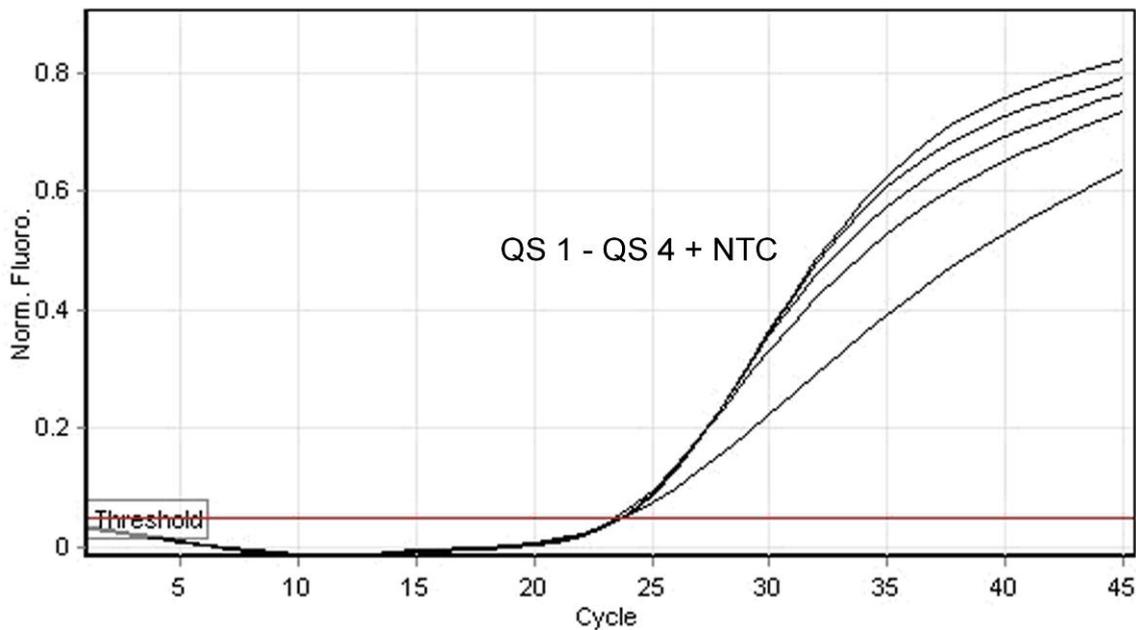


Figure 9. Detection of the internal control (IC) in fluorescence channel Cycling Orange with simultaneous amplification of the quantitation standards (VZV RG QS 1–4). NTC: No template control (negative control).

**A signal is detected in fluorescence channel Cycling Green.
The result of the analysis is positive: the sample contains VZV DNA.**

In this case, the detection of a signal in the Cycling Orange channel is dispensable, since high initial concentrations of VZV DNA (positive signal in the Cycling Green channel) can lead to a reduced or absent fluorescence signal of the internal control in the Cycling Orange channel (competition).

In fluorescence channel Cycling Green no signal is detected. At the same time, a signal from the internal control appears in the Cycling Orange channel.

In the sample no VZV DNA is detectable. It can be considered negative.

In the case of a negative VZV PCR, the detected signal of the internal control rules out the possibility of PCR inhibition.

No signal is detected in the Cycling Green or in the Cycling Orange channels.

No result can be concluded.

Information regarding error sources and their solution can be found in "Troubleshooting guide", page 18.

Troubleshooting guide

This troubleshooting guide may be helpful in solving any problems that may arise. For more information, see also the Frequently Asked Questions page at our Technical Support Center: www.qiagen.com/FAQ/FAQList.aspx. The scientists in QIAGEN Technical Services are always happy to answer any questions you may have about either the information and protocol in this handbook or sample and assay technologies (for contact information, see back cover or visit www.qiagen.com).

Comments and suggestions

No signal with positive controls (VZV RG QS 1–4) in fluorescence channel Cycling Green

- | | |
|--|--|
| a) The selected fluorescence channel for PCR data analysis does not comply with the protocol | For data analysis select the fluorescence channel Cycling Green for the analytical VZV PCR and the fluorescence channel Cycling Orange for the internal control PCR. |
| b) Incorrect programming of the temperature profile of the Rotor-Gene Instrument | Compare the temperature profile with the protocol. See "Protocol: PCR and data analysis", page 8. |

Comments and suggestions

- c) Incorrect configuration of the PCR Check your work steps by means of the pipetting scheme, and repeat the PCR, if necessary. See "Protocol: PCR and data analysis", page 8.
- d) The storage conditions for one or more kit components did not comply with the instructions given in "Reagent Storage and Handling" (page 7) Check the storage conditions and the expiration date (see the kit label) of the reagents and use a new kit, if necessary.
- e) The *artus* VZV RG PCR Kit has expired Check the storage conditions and the expiration date (see the kit label) of the reagents and use a new kit, if necessary.

Weak or no signal of the internal control of a negative CSF sample subjected to purification using the EZ1 DSP Virus Kit in fluorescence channel Cycling Orange and simultaneous absence of a signal in channel Cycling Green

- a) The PCR conditions do not comply with the protocol Check the PCR conditions (see above) and repeat the PCR with corrected settings, if necessary.
- b) The PCR was inhibited Make sure that you use the recommended isolation method and closely follow the manufacturer's instructions.
- c) DNA was lost during extraction If the internal control was added to the extraction, an absent signal of the internal control can indicate the loss of DNA during the extraction. Make sure that you use the recommended isolation method (see "DNA isolation", page 8) and closely follow the manufacturer's instructions.
- d) The storage conditions for one or more kit components did not comply with the instructions given in "Reagent Storage and Handling" (page 7) Check the storage conditions and the expiration date (see the kit label) of the reagents and use a new kit, if necessary.

Comments and suggestions

- e) The *artus* VZV RG PCR Kit has expired Check the storage conditions and the expiration date (see the kit label) of the reagents and use a new kit, if necessary.

Signals with the negative controls in fluorescence channel Cycling Green of the analytical PCR

- a) Contamination occurred during preparation of the PCR Repeat the PCR with new reagents in replicates.
If possible, close the PCR tubes directly after addition of the sample to be tested.
Make sure to pipet the positive controls last.
Make sure that work space and instruments are decontaminated at regular intervals.
- b) Contamination occurred during extraction Repeat the extraction and PCR of the sample to be tested using new reagents.
Make sure that work space and instruments are decontaminated at regular intervals.

Quality Control

In accordance with QIAGEN's ISO-certified Quality Management System, each lot of *artus* VZV RG PCR Kit is tested against predetermined specifications to ensure consistent product quality.

Limitations

The product is to be used by personnel specially instructed and trained in the in vitro diagnostics procedures only.

Strict compliance with the user manual is required for optimal PCR results.

Attention should be paid to expiration dates printed on the box and labels of all components. Do not use expired components.

Although rare, mutations within the highly conserved regions of the viral genome covered by the kit's primers and/or probe may result in underquantitation or failure to detect the presence of the virus in these cases. Validity and performance of the assay design are revised at regular intervals.

Performance Characteristics

Analytical sensitivity

To determine the analytical sensitivity of the *artus* VZV RG PCR Kit, a dilution series of VZV genomic DNA was set up from 10 to 0.001 copies/ μ l and analyzed on the Rotor-Gene 6000 in combination with the *artus* VZV RG PCR Kit. Testing was carried out on 3 different days on 8 replicates. The results were determined by a probit analysis. A graphical illustration of the probit analysis on the Rotor-Gene 6000 is shown in Figure 10. The analytical detection limit of the *artus* VZV RG PCR Kit in combination with the Rotor-Gene Q MDx/Q/6000 is 0.136 copies/ μ l ($p = 0.05$). This means that there is a 95% probability that 0.136 copies/ μ l will be detected.

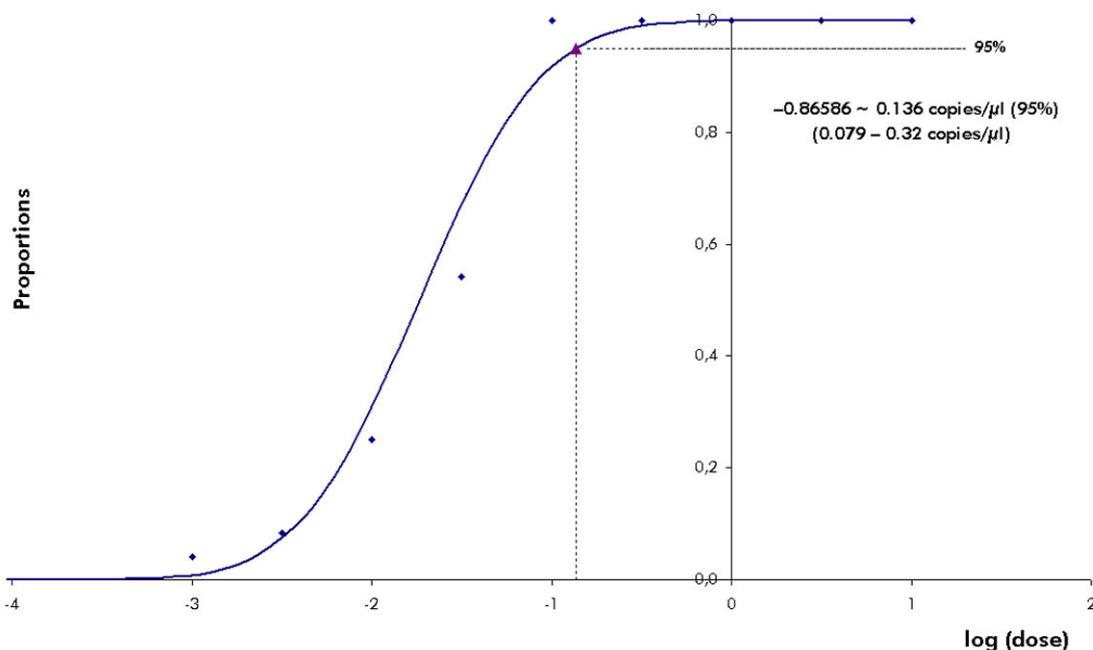


Figure 10. Probit analysis: VZV (Rotor-Gene 6000). Analytical sensitivity of the *artus* VZV RG PCR Kit on the Rotor-Gene 6000.

Specificity

The specificity of the *artus* VZV RG PCR Kit is first and foremost ensured by the selection of the primers and probes, as well as the selection of stringent reaction conditions. The primers and probes were checked for possible homologies to all published sequences in gene banks by sequence comparison analysis. The detectability of all relevant genotypes has thus been ensured.

Moreover, the specificity was validated with 30 different VZV negative CSF samples. These did not generate any signals with the VZV specific primers and probes, which are included in the VZV RG Master.

A potential cross-reactivity of the *artus* VZV RG PCR Kit was tested using the control group listed in Table 4. None of the tested pathogens has been reactive.

Table 4. Testing the specificity of the kit with potentially cross-reactive pathogens

Control group	VZV (Cycling Green)	Internal control (Cycling Orange)
Human herpesvirus 1 (herpes simplex virus 1)	–	+
Human herpesvirus 2 (herpes simplex virus 2)	–	+
Human herpesvirus 4 (Epstein-Barr virus)	–	+
Human herpesvirus 5 (cytomegalovirus)	–	+
Human herpesvirus 6A	–	+
Human herpesvirus 6B	–	+
Human herpesvirus 7	–	+
Human herpesvirus 8 (Kaposi's sarcoma-associated herpesvirus)	–	+
Hepatitis A virus	–	+
Hepatitis B virus	–	+
Hepatitis C virus	–	+
Human immunodeficiency virus (HIV)	–	+
Human T cell leukemia virus 1	–	+
Human T cell leukemia virus 2	–	+
Enterovirus	–	+
Parvovirus B19	–	+
West Nile virus	–	+

Precision

The precision data of the *artus* VZV RG PCR Kit have been collected by means of Rotor-Gene Instruments and allow the determination of the total variance of the assay. The total variance consists of the intra-assay variability (variability of multiple results of samples of the same concentration within one experiment), the inter-assay variability (variability of multiple results of the assay generated on different instruments of the same type by different operators within one laboratory) and the inter-batch variability (variability of multiple results of the assay using various batches). The data obtained were used to determine the standard deviation, the variance and the coefficient of variation for the pathogen specific and the internal control PCR.

Precision data of the *artus* VZV RG PCR have been collected using the quantitation standard of the lowest concentration (QS 4; 10 copies/ μ l). Testing was performed with 8 replicates. The precision data were calculated on basis of the C_T values of the amplification curves (C_T : threshold cycle, see Table 5, page 24). In addition, precision data for quantitative results in copies/ μ l were determined using the corresponding C_T values (see Table 6, page 24). Based on these results, the overall statistical spread of any given sample with the mentioned concentration is 0.45% (C_T) or 8.32% (concentration), and 2.81% (C_T) for the detection of the internal control. These values are based on the totality of all single values of the determined variabilities.

Robustness

The verification of the robustness allows the determination of the total failure rate of the *artus* VZV RG PCR Kit. 30 VZV negative samples of CSF were spiked with 0.4 copies/ μ l elution volume of VZV DNA (approximately threefold concentration of the analytical sensitivity limit). After extraction using the EZ1[®] DSP Virus Kit (see "DNA isolation", page 8), these samples were analyzed with the *artus* VZV RG PCR Kit. For all 30 samples the failure rate was 0%. In addition, the robustness of the internal control was assessed by purification and analysis of 30 VZV negative CSF samples. The total failure rate was 0%. Inhibitions were not observed. Thus, the robustness of the *artus* VZV RG PCR Kit is $\geq 99\%$.

Reproducibility

Reproducibility data permit a regular performance assessment of the *artus* VZV RG PCR Kit as well as an efficiency comparison with other products. These data are obtained by the participation in established proficiency programs.

Table 5. Precision data on basis of the C_T values

	Standard deviation	Variance	Coefficient of variation (%)
Intra-assay variability: VZV QS 4	0.08	0.01	0.26
Intra-assay variability: Internal control	0.04	0.002	0.17
Inter-assay variability: VZV QS 4	0.15	0.02	0.5
Inter-assay variability: Internal control	0.39	0.15	1.63
Inter-batch variability: VZV QS 4	0.1	0.01	0.34
Inter-batch variability: Internal control	0.66	0.43	2.65
Total variance: VZV QS 4	0.13	0.02	0.45
Total variance: Internal control	0.68	0.47	2.81

Table 6. Precision data on basis of the quantitative results (in copies/ μ l)

	Standard deviation	Variance	Coefficient of variation (%)
Intra-assay variability: VZV QS 4	0.5	0.25	5.46
Inter-assay variability: VZV QS 4	0.85	0.72	8.72
Inter-batch variability: VZVQS 4	0.75	0.56	7.67
Total variance: VZV QS 4	0.81	0.66	8.32

References

QIAGEN maintains a large, up-to-date online database of scientific publications utilizing QIAGEN products. Comprehensive search options allow you to find the articles you need, either by a simple keyword search or by specifying the application, research area, title, etc.

For a complete list of references, visit the QIAGEN Reference Database online at www.qiagen.com/RefDB/search.asp or contact QIAGEN Technical Services or your local distributor.

Symbols

 Σ	Contains reagents sufficient for <N> tests
	Use by
IVD	In vitro diagnostic medical device
REF	Catalog number
LOT	Lot number
MAT	Material number
COMP	Components
CONT	Contains
NUM	Number
GTIN	Global Trade Item Number
	Temperature limitation
	Manufacturer
	Consult instructions for use

Contact Information

For technical assistance and more information, please see our Technical Support Center at www.qiagen.com/Support or call one of the QIAGEN Technical Service Departments or local distributors (see back cover or visit www.qiagen.com).

Ordering Information

Product	Contents	Cat. no.
<i>artus</i> VZV RG PCR Kit (24)	For 24 reactions: Master, 4 Quantitation Standards, Internal Control, Magnesium Solution, Water (PCR grade)	4502263
<i>artus</i> VZV RG PCR Kit (96)	For 96 reactions: Master, 4 Quantitation Standards, Internal Control, Magnesium Solution, Water (PCR grade)	4502265
EASY<i>artus</i> VZV RG PCR Kits — for fully CE-IVD-compliant integrated automated sample purification and pathogen detection		
EASY <i>artus</i> VZV RG PCR Kit 1	For 48 viral nucleic acid preps and 24 assays: 1 x EZ1 DSP Virus Kit, 1 x <i>artus</i> VZV RG PCR Kit (24)	EA10223
EASY <i>artus</i> VZV RG PCR Kit 2	For 48 viral nucleic acid preps and 48 assays: 1 x EZ1 DSP Virus Kit, 2 x <i>artus</i> VZV RG PCR Kit (24)	EA10224
EZ1 DSP Virus Kit — for automated, simultaneous purification of viral DNA and RNA from 1–14 human plasma, serum, or CSF samples		
EZ1 DSP Virus Kit (48)	For 48 viral nucleic acid preps: Prefilled Reagent Cartridges, Disposable Tip Holders, Disposable Filter-Tips, Sample Tubes, Elution Tubes, Buffers, Carrier RNA	62724
Rotor-Gene Q MDx and accessories		
Rotor-Gene Q MDx 5plex Platform	Real-time PCR cycler with 5 channels (green, yellow, orange, red, crimson), laptop computer, software, accessories: includes 1-year warranty on parts and labor, installation and training not included	9002022

Product	Contents	Cat. no.
Rotor-Gene Q MDx 5plex System	Real-time PCR cycler with 5 channels (green, yellow, orange, red, crimson), laptop computer, software, accessories: includes 1-year warranty on parts and labor, installation and training	9002023
Rotor-Gene Q MDx 5plex HRM Platform	Real-time PCR cycler and High Resolution Melt analyzer with 5 channels (green, yellow, orange, red, crimson) plus HRM channel, laptop computer, software, accessories: includes 1-year warranty on parts and labor, installation and training not included	9002032
Rotor-Gene Q MDx 5plex HRM System	Real-time PCR cycler and High Resolution Melt analyzer with 5 channels (green, yellow, orange, red, crimson) plus HRM channel, laptop computer, software, accessories: includes 1-year warranty on parts and labor, installation and training	9002033
Rotor-Gene Q MDx 6plex Platform	Real-time PCR instrument with 6 channels (blue, green, yellow, orange, red, crimson), including laptop computer, software, accessories: includes 1-year warranty on parts and labor, installation and training not included	9002042
Rotor-Gene Q MDx 6plex System	Real-time PCR instrument with 6 channels (blue, green, yellow, orange, red, crimson), including laptop computer, software, accessories: includes 1-year warranty on parts and labor, installation and training	9002043
Loading Block 72 x 0.1 ml Tubes	Aluminum block for manual reaction setup with a single-channel pipet in 72 x 0.1 ml tubes	9018901
Loading Block 96 x 0.2 ml Tubes	Aluminum block for manual reaction set-up in a standard 8 x 12 array using 96 x 0.2 ml tubes	9018905

Product	Contents	Cat. no.
Strip Tubes and Caps, 0.1 ml (250)	250 strips of 4 tubes and caps for 1000 reactions	981103
Strip Tubes and Caps, 0.1 ml (2500)	10 x 250 strips of 4 tubes and caps for 10,000 reactions	981106
PCR Tubes, 0.2 ml (1000)	1000 thin-walled tubes for 1000 reactions	981005
PCR Tubes, 0.2 ml (10000)	10 x 1000 thin-walled tubes for 10,000 reactions	981008

For up-to-date licensing information and product-specific disclaimers, see the respective QIAGEN kit handbook or user manual. QIAGEN kit handbooks and user manuals are available at www.qiagen.com or can be requested from QIAGEN Technical Services or your local distributor.

This page intentionally left blank

The purchase of this product allows the purchaser to use it for the performance of diagnostic services for human in vitro diagnostics. No general patent or other license of any kind other than this specific right of use from purchase is granted hereby.

Trademarks: QIAGEN®, *artus*®, EASY*artus*®, EZ1®, Rotor-Gene® (QIAGEN Group).

Limited License Agreement

Use of this product signifies the agreement of any purchaser or user of the *artus* VZV RG PCR Kit to the following terms:

1. The *artus* VZV RG PCR Kit may be used solely in accordance with the *artus* VZV RG PCR Kit Handbook and for use with components contained in the Kit only. QIAGEN grants no license under any of its intellectual property to use or incorporate the enclosed components of this Kit with any components not included within this Kit except as described in the *artus* VZV RG PCR Kit Handbook and additional protocols available at www.qiagen.com.
2. Other than expressly stated licenses, QIAGEN makes no warranty that this Kit and/or its use(s) do not infringe the rights of third-parties.
3. This Kit and its components are licensed for one-time use and may not be reused, refurbished, or resold.
4. QIAGEN specifically disclaims any other licenses, expressed or implied other than those expressly stated.
5. The purchaser and user of the Kit agree not to take or permit anyone else to take any steps that could lead to or facilitate any acts prohibited above. QIAGEN may enforce the prohibitions of this Limited License Agreement in any Court, and shall recover all its investigative and Court costs, including attorney fees, in any action to enforce this Limited License Agreement or any of its intellectual property rights relating to the Kit and/or its components.

For updated license terms, see www.qiagen.com.

© 2009–2014 QIAGEN, all rights reserved.

www.qiagen.com

Australia ■ Orders 1-800-243-800 ■ Fax 03-9840-9888 ■ Technical 1-800-243-066

Austria ■ Orders 0800-28-10-10 ■ Fax 0800-28-10-19 ■ Technical 0800-28-10-11

Belgium ■ Orders 0800-79612 ■ Fax 0800-79611 ■ Technical 0800-79556

Brazil ■ Orders 0800-557779 ■ Fax 55-11-5079-4001 ■ Technical 0800-557779

Canada ■ Orders 800-572-9613 ■ Fax 800-713-5951 ■ Technical 800-DNA-PREP (800-362-7737)

China ■ Orders 86-21-3865-3865 ■ Fax 86-21-3865-3965 ■ Technical 800-988-0325

Denmark ■ Orders 80-885945 ■ Fax 80-885944 ■ Technical 80-885942

Finland ■ Orders 0800-914416 ■ Fax 0800-914415 ■ Technical 0800-914413

France ■ Orders 01-60-920-926 ■ Fax 01-60-920-925 ■ Technical 01-60-920-930 ■ Offers 01-60-920-928

Germany ■ Orders 02103-29-12000 ■ Fax 02103-29-22000 ■ Technical 02103-29-12400

Hong Kong ■ Orders 800 933 965 ■ Fax 800 930 439 ■ Technical 800 930 425

Ireland ■ Orders 1800 555 049 ■ Fax 1800 555 048 ■ Technical 1800 555 061

Italy ■ Orders 800-789-544 ■ Fax 02-334304-826 ■ Technical 800-787980

Japan ■ Telephone 03-6890-7300 ■ Fax 03-5547-0818 ■ Technical 03-6890-7300

Korea (South) ■ Orders 080-000-7146 ■ Fax 02-2626-5703 ■ Technical 080-000-7145

Luxembourg ■ Orders 8002-2076 ■ Fax 8002-2073 ■ Technical 8002-2067

Mexico ■ Orders 01-800-7742-639 ■ Fax 01-800-1122-330 ■ Technical 01-800-7742-436

The Netherlands ■ Orders 0800-0229592 ■ Fax 0800-0229593 ■ Technical 0800-0229602

Norway ■ Orders 800-18859 ■ Fax 800-18817 ■ Technical 800-18712

Singapore ■ Orders 1800-742-4362 ■ Fax 65-6854-8184 ■ Technical 1800-742-4368

Spain ■ Orders 91-630-7050 ■ Fax 91-630-5145 ■ Technical 91-630-7050

Sweden ■ Orders 020-790282 ■ Fax 020-790582 ■ Technical 020-798328

Switzerland ■ Orders 055-254-22-11 ■ Fax 055-254-22-13 ■ Technical 055-254-22-12

UK ■ Orders 01293-422-911 ■ Fax 01293-422-922 ■ Technical 01293-422-999

USA ■ Orders 800-426-8157 ■ Fax 800-718-2056 ■ Technical 800-DNA-PREP (800-362-7737)

