
November 2020

RNeasy® Fibrous Tissue Mini Handbook

For purification of total RNA
from heart, skeletal muscle,
aorta and other fiber-rich
tissues

Contents

- Kit Contents 3
- Storage 4
- Intended Use 4
- Safety Information..... 5
- Quality Control..... 5
- Introduction 6
 - Principle and procedure 6
 - Automated purification of RNA on QIAcube Instruments..... 8
- Equipment and Reagents to Be Supplied by User 9
- Important Notes..... 10
 - Determining the amount of starting material 10
 - Handling and storing starting material 12
 - Disrupting and homogenizing starting material 13
- Protocol: Purification of Total RNA using the RNeasy Fibrous Tissue Mini Kit..... 15
- Troubleshooting Guide 22
- Appendix A: General Remarks on Handling RNA..... 25
- Appendix B: Storage, Quantification and Determination of Quality of RNA..... 28
- Appendix C: DNase Digestion of RNA Eluates using the RNase-Free DNase Set 32
- Ordering Information 34
- Document Revision History 36

Kit Contents

RNeasy Fibrous Tissue Mini Kit	(50)
Catalog no.	74704
No. of preps	50
RNeasy Mini Spin Columns (each in a 2 ml collection tube)	50
Collection Tubes (1.5 ml)	50
Collection Tubes (2 ml)	50
Proteinase K	2 ml
Buffer RLT*	45 ml
Buffer RW1 *	45 ml
Buffer RPE† (concentrate)	11 ml
RNase-Free Water	4 x 10 ml
RNase-Free DNase Set:	
RNase-Free DNase I (lyophilized)	1500 units
Buffer RDD	2 x 2 ml
RNase-Free Water	1.5 ml
Quick-Start Protocol	1

* Contains a guanidine salt. Not compatible with disinfectants containing bleach. See page 5 for safety information.

† Before using for the first time, add 4 volumes of ethanol (96–100%) as indicated on the bottle to obtain a working solution.

Storage

The RNeasy Fibrous Tissue Mini Kit is shipped at ambient temperature and should be stored dry at room temperature (15–25°C). The RNase-Free DNase Set should be stored immediately upon receipt at 2–8°C. All components are stable for at least 9 months under these conditions, if not otherwise stated on the label.

The ready-to-use proteinase K included in the kit is dissolved in a specially formulated storage buffer. The proteinase K is stable for up to 1 year after delivery when stored at room temperature. To prolong the lifetime of the proteinase K, we recommend storage at 2–8°C.

Intended Use

The RNeasy Fibrous Tissue Mini Kit is intended for molecular biology applications. This product is not intended for the diagnosis, prevention or treatment of a disease.

QIAcube® Connect is designed to perform fully automated purification of nucleic acids and proteins in molecular biology applications. The system is intended for use by professional users trained in molecular biological techniques and the operation of QIAcube Connect.

All due care and attention should be exercised in the handling of the products. We recommend all users of QIAGEN® products to adhere to the NIH guidelines that have been developed for recombinant DNA experiments or to other applicable guidelines.

Safety Information

When working with chemicals, always wear a suitable lab coat, disposable gloves and protective goggles. For more information, please consult the appropriate safety data sheets (SDSs). These are available online in convenient and compact PDF format at **www.qiagen.com/safety** where you can find, view and print the SDS for each QIAGEN kit and kit component.

CAUTION



DO NOT add bleach or acidic solutions directly to the sample preparation waste

Buffer RLT contains guanidine thiocyanate and Buffer RW1 contains a small amount of guanidine thiocyanate. Guanidine salts can form highly reactive compounds when combined with bleach. If liquid containing these buffers is spilt, clean with suitable laboratory detergent and water. If the spilt liquid contains potentially infectious agents, clean the affected area first with laboratory detergent and water, and then with 1% (v/v) sodium hypochlorite.

Quality Control

In accordance with QIAGEN's ISO-certified Quality Management System, each lot of RNeasy Fibrous Tissue Mini Kit is tested against predetermined specifications to ensure consistent product quality.

Introduction

The RNeasy Fibrous Tissue Mini Kit is designed for optimal lysis of fiber-rich tissues and purification of high-quality total RNA >200 nt.


Principle and procedure

Total RNA purification from fibrous tissues, such as skeletal muscle, heart and aorta tissue can be difficult due to the abundance of contractile proteins, connective tissue and collagen. The RNeasy Fibrous Tissue Mini Kit is supplied with proteinase K, which removes these proteins.

Tissue samples are first lysed in Buffer RLT and then diluted before being treated with proteinase K. Debris is pelleted by centrifugation, and the supernatant is removed. The supernatant is mixed with ethanol and then centrifuged through an RNeasy Mini spin column, where RNA binds to the silica membrane. Traces of DNA that may co-purify with the RNA are removed by DNase treatment on the silica membrane. DNase and any contaminants are efficiently washed away, and high-quality total RNA is eluted in RNase-free water. The RNeasy Fibrous Tissue Mini Kit purifies RNA from up to 30 mg tissue (flowchart, next page).

With the RNeasy Fibrous Tissue Mini Kit, all RNA molecules longer than 200 nucleotides are purified. The procedure provides enrichment for mRNA since most RNAs <200 nucleotides (such as 5.8S rRNA, 5S rRNA and tRNAs, which together comprise 15–20% of total RNA) are selectively excluded. For purification of small RNA, including microRNA, from tissues and cells, we recommend using miRNeasy Kits.

RNeasy Fibrous Tissue Mini Procedure

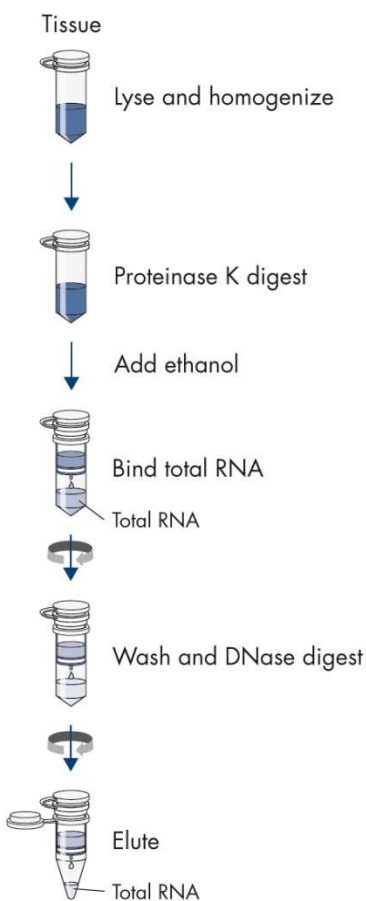

Automated purification of RNA on QIAcube Instruments

Purification of RNA can be fully automated on QIAcube Connect or the classic QIAcube. The innovative QIAcube instruments use advanced technology to process QIAGEN spin columns, enabling seamless integration of automated, low-throughput sample prep into your laboratory workflow. Sample preparation using QIAcube instruments follows the same steps as the manual procedure (i.e., lyse, bind, wash and elute), enabling you to continue using the RNeasy Fibrous Tissue Mini Kit for purification of high-quality RNA.

QIAcube instruments are preinstalled with protocols for purification of plasmid DNA, genomic DNA, RNA, viral nucleic acids and proteins, plus DNA and RNA cleanup. The range of protocols available is continually expanding and additional QIAGEN protocols can be downloaded free of charge at www.qiagen.com/qiacubeprotocols.



QIAcube Connect.

Equipment and Reagents to Be Supplied by User

When working with chemicals, always wear a suitable lab coat, disposable gloves and protective goggles. For more information, consult the appropriate safety data sheets (SDSs), available from the product supplier.

- 14.3 M β -mercaptoethanol (β -ME) (commercially available solutions are usually 14.3 M), alternatively dithiothreitol (DTT, 2 M stock solution)
- Ethanol (96–100%)*
- Sterile, RNase-free pipette tips
- Disposable gloves
- Water bath or heating block capable of reaching 55°C
- Equipment for tissue disruption and homogenization (see page 13). We recommend either the TissueRuptor® II with TissueRuptor Disposable Probes or the TissueLyser II (see Ordering Information, page 34)
- For stabilization of RNA in tissues (see “Handling and storing starting material”, page 12): RNAlater® Tissue Reagent (cat. no. 76104 or 76106) or Allprotect® Tissue Reagent (cat. no. 76405) or liquid nitrogen and dry ice
- 1.5 ml or 2 ml microcentrifuge tubes
- Microcentrifuge (with rotor for 2 ml tubes)

* Do not use denatured alcohol, which contains other substances, such as methanol or methyl ethyl ketone.

Important Notes

Determining the amount of starting material

It is essential to use the correct amount of starting material to obtain optimal RNA yield and purity. The maximum amount that can be used is determined by:

- The type of tissue and its RNA content
- The volume of Buffer RLT required for efficient lysis
- The RNA binding capacity of the RNeasy Mini spin column

When processing samples containing high amounts of RNA, less than the maximum amount of starting material shown in Table 1 (next page) should be used, so that the RNA binding capacity of the RNeasy Mini spin column is not exceeded.

When processing samples containing low amounts of RNA, the maximum amount of starting material shown in Table 1 can be used. However, even though the RNA binding capacity of the RNeasy Mini spin column is not reached, the maximum amount of starting material must not be exceeded. Otherwise, lysis will be incomplete and cellular debris may interfere with the binding of RNA to the RNeasy Mini spin column membrane, resulting in lower RNA yield and purity.

More information on using the correct amount of starting material is given in the protocols. Table 2 (next page) shows expected RNA yields from various sources.

Table 1. RNeasy Mini spin column specifications

Specification	RNeasy Mini spin column
Maximum binding capacity	100 µg RNA
Maximum loading volume	700 µl
Minimum elution volume	30 µl
Maximum amount of starting tissue	≤30 mg

Note: If the binding capacity of the RNeasy Mini spin column is exceeded, RNA yields will not be consistent and may be reduced. If lysis of the starting material is incomplete, RNA yields will be lower than expected, even if the binding capacity of the RNeasy Mini spin column is not exceeded.

Table 2. Typical yields of total RNA

Mouse/rat tissue (10 mg)	Yield of total RNA (µg)*
Heart	8–12
Aorta	8–12
Trachea	8–12
Esophagus	8–12
Muscle	5–10
Skin	4–8
Eye	8–12
Ear	10–15

* Amounts can vary due to factors, such as species and developmental stage. Since the RNeasy Fibrous Tissue Mini Kit enriches for mRNA and other RNA species >200 nucleotides, the total RNA yield does not include 5S rRNA, tRNA and other low-molecular-weight RNAs, which make up 15–20% of total cellular RNA.

Handling and storing starting material

RNA in harvested tissue is not protected until the sample is treated with RNAlprotect Tissue Reagent, flash-frozen or disrupted and homogenized in the presence of RNase-inhibiting or denaturing reagents. If unprotected, unwanted changes in the gene expression profile will occur. It is therefore important that tissue samples are immediately frozen in liquid nitrogen and stored at -90°C to -65°C or immediately immersed in RNAlprotect Tissue Reagent or AllProtect Tissue Reagent at room temperature ($15\text{--}25^{\circ}\text{C}$) or immediately frozen in liquid nitrogen and stored at -90°C to -65°C . Otherwise, unwanted changes in the gene expression profile will occur

The procedures for tissue harvesting and RNA protection should be carried out as quickly as possible. Frozen tissue samples should not be allowed to thaw during handling or weighing. After disruption and homogenization in Buffer RLT (lysis buffer), samples can be stored at -90°C to -65°C for several months. Storage times differ for different tissue types and have not been established for all possible tissues.

Disrupting and homogenizing starting material

Efficient disruption and homogenization of the starting material is an absolute requirement for all total RNA purification procedures. Disruption and homogenization are two distinct steps:

- **Disruption:** Complete disruption of plasma membranes of cells and organelles is absolutely required to release all the RNA contained in the sample. Incomplete disruption results in significantly reduced RNA yields.
- **Homogenization:** Homogenization is necessary to reduce the viscosity of the lysates produced by disruption. Homogenization shears high-molecular-weight genomic DNA and other high-molecular-weight cellular components to create a homogeneous lysate. Incomplete homogenization results in inefficient binding of RNA to the RNeasy Mini spin column membrane and therefore significantly reduced RNA yields.

Disruption and homogenization of tissue samples can be carried out rapidly and efficiently using either the TissueRuptor II (for processing samples individually) or the TissueLyser (for processing multiple samples simultaneously). Disruption and homogenization with the TissueRuptor II or TissueLyser generally result in higher RNA yields than with other methods.

Disruption and homogenization using the TissueRuptor II

The TissueRuptor II is a rotor–stator homogenizer that thoroughly disrupts and simultaneously homogenizes single tissue samples in the presence of lysis buffer in 15–90 seconds, depending on the toughness and size of the sample. The blade of the TissueRuptor disposable probe rotates at a very high speed, causing the sample to be disrupted and homogenized by a combination of turbulence and mechanical shearing.

For guidelines on using the TissueRuptor II, refer to the *TissueRuptor II Handbook*. For other rotor–stator homogenizers, refer to suppliers' guidelines.

Disruption and homogenization using the TissueLyser II

In bead-milling, tissues can be disrupted by rapid agitation in the presence of beads and lysis buffer. Disruption and simultaneous homogenization occur by the shearing and crushing action of the beads as they collide with the cells. The TissueLyser II disrupts and homogenizes up to 48 tissue samples simultaneously when used in combination with the TissueLyser Adapter Set 2 x 24, which holds 48 x 2 ml microcentrifuge tubes containing stainless steel beads of 5 mm mean diameter. For guidelines on using the TissueLyser II, refer to the *TissueLyser Handbook*. For other bead mills, refer to suppliers' guidelines.

Note: Tungsten carbide beads react with Buffer RLT and must not be used to disrupt and homogenize tissues.

The TissueLyser II can also disrupt and homogenize up to 192 tissue samples simultaneously when used in combination with the TissueLyser Adapter Set 2 x 96, which holds 192 x 1.2 ml microcentrifuge tubes containing stainless steel beads of 5 mm mean diameter. In this case, we recommend using the RNeasy 96 Universal Tissue Kit (cat. no. 74881), which provides high-throughput RNA purification from all types of tissue – including fiber-rich tissues – in 96-well format.

Protocol: Purification of Total RNA using the RNeasy Fibrous Tissue Mini Kit

Determining the correct amount of starting material

It is essential to use the correct amount of tissue to obtain optimal RNA yield and purity. A maximum of 30 mg tissue can generally be processed. For most tissues, the RNA binding capacity of the RNeasy Mini spin column and the lysing capacity of Buffer RLT and proteinase K will not be exceeded by this amount. Average RNA yields from various tissues are given in Table 2 (page 11).

If there is no information about the nature of your starting material, we recommend starting with no more than 10 mg tissue. Depending on RNA yield and purity, it may be possible to use up to 30 mg tissue in subsequent preparations.

IMPORTANT: Do not overload the RNeasy Mini spin column, as this will significantly reduce RNA yield and quality.

Weighing tissue is the most accurate way to quantify the amount of starting material. As a guide, a 3 mm cube (27 mm³) of most animal tissues weighs 25–35 mg.

Important points before starting

- If using the RNeasy Fibrous Tissue Mini Kit for the first time, read “Important Notes” (page 10).
- If working with RNA for the first time, read “Appendix A: General Remarks on Handling RNA”, page 25).
- If using the TissueRuptor II, ensure that you are familiar with operating it by referring to the *TissueRuptor II User Manual* and *TissueRuptor II Handbook*.

- If using the TissueLyser II, ensure that you are familiar with operating it by referring to the operating instructions and *TissueLyser Handbook*.
- Since the RNase-inactivating Buffer RLT must be diluted to permit proteinase K digestion, this protocol should not be used for tissues rich in RNases, such as pancreas or intestine.
- Fresh, frozen or RNAprotect-stabilized tissues can be used. If freezing tissues, flash-freeze in liquid nitrogen and immediately transfer to -90°C to -65°C , where they can be stored for several months. Do not allow tissues to thaw during weighing or handling prior to disruption in Buffer RLT. Homogenized tissue lysates from step 4 can also be stored at -90°C to -65°C for several months. Incubate frozen lysates at 37°C in a water bath until completely thawed and salts are dissolved before continuing with step 5. Avoid prolonged incubation, which may compromise RNA integrity.
- **Important:** Do not vortex reconstituted DNase I. DNase I is especially sensitive to physical denaturation. Mixing should only be carried out by gently inverting the tube.
- Buffer RLT may form a precipitate upon storage. If necessary, redissolve by warming, and then place at room temperature ($15\text{--}25^{\circ}\text{C}$).

Things to do before starting

- β -mercaptoethanol (β -ME) must be added to Buffer RLT Plus before use. Add $10\text{ }\mu\text{l}$ β -ME per 1 ml Buffer RLT. Dispense in a fume hood and wear appropriate protective clothing. Buffer RLT is stable at room temperature ($15\text{--}25^{\circ}\text{C}$) for 1 month after addition of β -ME. Alternatively, add $20\text{ }\mu\text{l}$ 2 M dithiothreitol (DTT) per 1 ml Buffer RLT. The stock solution of 2 M DTT in water should be prepared fresh or frozen in single-use aliquots. Buffer RLT containing DTT can be stored at room temperature for up to 1 month.
- Buffer RPE is supplied as a concentrate. Before using for the first time, add 4 volumes of ethanol ($96\text{--}100\%$) as indicated on the bottle to obtain a working solution.

- Prepare DNase I stock solution before using the RNase-Free DNase Set for the first time. Dissolve the lyophilized DNase I (1500 Kunitz units) in 550 µl of the RNase-free water provided in the RNase-Free DNase Set box. To avoid loss of DNase I, do not open the vial. Inject RNase-free water into the vial using an RNase-free needle and syringe. Mix gently by inverting the vial. Do not vortex.

For long-term storage of DNase I, remove the stock solution from the glass vial, divide it into single-use aliquots, and store at -30°C to -15°C for up to 9 months. Thawed aliquots can be stored at $2-8^{\circ}\text{C}$ for up to 6 weeks. Do not refreeze the aliquots after thawing.

Procedure

1. Heat a water bath or heating block to 55°C for proteinase K digestion in step 4b.
2. If using the TissueLyser II, add one stainless steel bead (5 mm mean diameter) per 2 ml microcentrifuge tube (not supplied). If working with tissues that are not stabilized in RNAlater-Reagent, place the tubes on dry ice.
3. Excise the tissue sample from the animal or remove it from storage. Determine the amount of tissue. Do not use more than 30 mg. Proceed immediately to step 4.

Note: Weighing tissue is the most accurate way to determine the amount.

Note: If the tissue sample was stored in RNAlater Tissue Reagent, remove it from the reagent using forceps and be sure to remove any excess reagent or crystals that may have formed.

Note: RNA in harvested tissues is not protected until the tissues are treated with RNAlater Tissue Reagent, flash-frozen or disrupted and homogenized in step 4. Frozen tissues should not be allowed to thaw during handling. The relevant procedures should be carried out as quickly as possible.

4. Disrupt the tissue and homogenize the lysate using **EITHER** the TissueRuptor II (follow steps 4a and 4b) **OR** the TissueLyser II (follow steps 4c to 4h).

See “Disrupting and homogenizing starting material”, page 13, for more details on disruption and homogenization.

Note: Ensure that β -ME is added to Buffer RLT before use (see “Things to do before starting”, page 16).

Note: Incomplete homogenization leads to significantly reduced RNA yields and can cause clogging of the RNeasy Mini spin column. Homogenization with the TissueRuptor II or TissueLyser II generally results in higher RNA yields than with other methods.

Disruption and homogenization using the TissueRuptor II

- 4a. Place the tissue in a suitably sized vessel. Add 300 μ l Buffer RLT.

Generally, round-bottomed tubes allow more efficient disruption and homogenization than conical-bottomed tubes.

- 4b. Place the tip of the disposable probe into the vessel and operate the TissueRuptor II at full speed until the lysate is uniformly homogeneous (usually 20–40 s). Proceed to step 5.

Note: To avoid damage to the TissueRuptor II and disposable probe during operation, make sure the tip of the probe remains submerged in the buffer.

Disruption and homogenization using the TissueLyser II

- 4c. Place the tissues in the tubes prepared in step 2.
- 4d. If the tubes were stored on dry ice, place them at room temperature (15–25°C). Then immediately add 300 μ l Buffer RLT per tube.
- 4e. Place the tubes in the TissueLyser Adapter Set 2 x 24.
- 4f. Operate the TissueLyser II for 2 min at 20 Hz.

Note: The time depends on the tissue being processed and can be extended until the tissue is completely homogenized.

4g. Disassemble the adapter set, rotate the rack of tubes so that the tubes nearest to the TissueLyser II are now outermost, and reassemble the adapter set. Operate the TissueLyser II for another 2 min at 20 Hz.

Note: Rearranging the tubes allows even homogenization.

4h. Carefully pipet the lysates into new microcentrifuge tubes (not supplied). Proceed to step 5.

Important: Do not reuse the stainless-steel beads.

Preparation of total RNA

5. Add 590 μ l RNase-free water to the lysate. Then add 10 μ l proteinase K solution and mix thoroughly by pipetting.
6. Incubate at 55°C for 10 min.
7. Centrifuge at 15–25°C for 3 min at 10,000 $\times g$.

A small pellet of tissue debris will form, sometimes accompanied by a thin layer or film on top of the supernatant.

8. Pipet the supernatant (approximately 900 μ l) into a new 1.5 ml or 2 ml microcentrifuge tube (not supplied).

Avoid transferring any of the pellet. If this is unavoidable, a small amount of pelleted debris may be carried over without affecting the RNeasy procedure. Hold the pipette tip under the thin layer or film on top of the supernatant, if present. This layer will usually adhere to the outside of the pipette tip and should not be transferred.

9. Add 0.5 volumes (usually 450 μ l) of ethanol (96–100%) to the cleared lysate. Mix well by pipetting. Do not centrifuge.

Precipitates may be visible after addition of ethanol. This does not affect the procedure.

10. Transfer 700 μ l of the sample, including any precipitate that may have formed, to an RNeasy Mini spin column placed in a 2 ml collection tube. Close the lid gently, and centrifuge at 15–25°C for 15 s at $\geq 8000 \times g$ ($\geq 10,000$ rpm). Discard the flow-through.*
Reuse the collection tube in step 11.
11. Repeat step 10 using the remainder of the sample. Discard the flow-through.*
Reuse the collection tube in step 12.
12. Add 350 μ l Buffer RW1 to the RNeasy Mini spin column. Close the lid gently and centrifuge at 15–25°C for 15 s at $\geq 8000 \times g$ ($\geq 10,000$ rpm) to wash the membrane. Discard the flow-through.
Reuse the collection tube in step 15.
- Optional:** If on-column DNase digestion is not desired, add 700 μ l Buffer RW1 instead, centrifuge for 15 s at $\geq 8000 \times g$, and discard the flow-through* (but not the collection tube). Proceed to step 16.
13. Add 10 μ l DNase I stock solution to 70 μ l Buffer RDD. Mix by gently inverting the tube, and centrifuge briefly to collect residual liquid from the sides of the tube.
Note: DNase I is especially sensitive to physical denaturation. Mixing should only be carried out by gently inverting the tube. Do not vortex.
14. Add the DNase I incubation mix (80 μ l) directly to the RNeasy Mini spin column membrane and place on the benchtop (15–25°C) for 15 min.
Note: Be sure to add the DNase I incubation mix directly to the RNeasy Mini spin column membrane. DNase digestion will be incomplete if part of the mix sticks to the walls or the O-ring of the spin column.
15. Add 350 μ l Buffer RW1 to the RNeasy Mini spin column. Close the lid gently and centrifuge for 15 s at $\geq 8000 \times g$ ($\geq 10,000$ rpm) at 15–25°C. Discard the flow-through.*
Reuse the collection tube in step 16.

* Flow-through contains Buffer RLT or Buffer RW1 and is therefore not compatible with bleach. See page 6 for safety information.

16. Add 500 µl Buffer RPE to the RNeasy Mini spin column. Close the lid gently and centrifuge at 15–25°C for 15 s at $\geq 8000 \times g$ ($\geq 10,000$ rpm) to wash the membrane. Discard the flow-through.

Reuse the collection tube in step 17.

Note: Buffer RPE is supplied as a concentrate. Ensure that ethanol is added to Buffer RPE before use (see “Things to do before starting”, page 16).

17. Add 500 µl Buffer RPE to the RNeasy Mini spin column. Close the lid gently and centrifuge at 15–25°C for 2 min at $\geq 8000 \times g$ ($\geq 10,000$ rpm) to wash the membrane.

The long centrifugation dries the spin column membrane, ensuring that no ethanol is carried over during RNA elution. Residual ethanol may interfere with downstream reactions.

Note: After centrifugation, carefully remove the RNeasy Mini spin column from the collection tube so that the column does not contact the flow-through. Otherwise, carryover of ethanol will occur.

18. **Optional:** Place the RNeasy Mini spin column in a new 2 ml collection tube (supplied) and discard the old collection tube with the flow-through. Close the lid gently and centrifuge at full speed for 1 min.

Perform this step to eliminate any possible carryover of Buffer RPE, or if residual flow-through remains on the outside of the RNeasy Mini spin column after step 17.

19. Place the RNeasy Mini spin column in a new 1.5 ml collection tube (supplied). Add 30–50 µl RNase-free water directly to the RNeasy Mini spin column membrane. Close the lid gently. To elute the RNA, centrifuge for 1 min at $\geq 8000 \times g$ ($\geq 10,000$ rpm) at 15–25°C.

20. Repeat step 19 using another 30–50 µl RNase-free water, or using the eluate from step 11 (if high RNA concentration is required). Reuse the collection tube from step 19. If the expected RNA yield is >30 µg, there is no need to repeat step 20.

If using the eluate from step 19, the RNA yield will be 15–30% less than that obtained using a second volume of RNase-free water, but the final RNA concentration will be higher.

Troubleshooting Guide

This troubleshooting guide may be helpful in solving any problems that may arise. For more information, see also the Frequently Asked Questions page at our Technical Support Center: www.qiagen.com/FAQ/FAQList.aspx. The scientists in QIAGEN Technical Services are always happy to answer any questions you may have about either the information and/or protocols in this handbook or sample and assay technologies (for contact information, visit www.qiagen.com).

Comments and suggestions

Clogged RNeasy Mini spin column

- | | |
|---|---|
| a) Inefficient disruption and/or homogenization | See “Disrupting and homogenizing starting material” (page 13) for details on disruption and homogenization methods.

Increase <i>g</i> -force and centrifugation time, if necessary.

In subsequent preparations, reduce the amount of starting material (see page 10 and protocol) and/or increase the homogenization time. |
| b) Too much starting material | In subsequent preparations, reduce the amount of starting material. It is essential to use the correct amount of starting material (see page 10 and protocol). |
| c) Centrifugation temperature too low | The centrifugation temperature should be 15–25°C. Some centrifuges may cool to below 20°C even when set at 20°C. This can cause formation of precipitates that can clog the RNeasy Mini spin column. If this happens, set the centrifugation temperature to 25°C. Warm the ethanol-containing lysate to 37°C before transferring it to the RNeasy Mini spin column. |

Low RNA yield

- | | |
|--|--|
| a) Inefficient disruption and/or homogenization | See “Disrupting and homogenizing starting material” (page 13) for details on disruption and homogenization methods.

Increase <i>g</i> -force and centrifugation time, if necessary.

In subsequent preparations, reduce the amount of starting material (see page 10 and protocol) and/or increase the homogenization time. |
| b) Too much starting material | In subsequent preparations, reduce the amount of starting material. It is essential to use the correct amount of starting material (see page 10 and protocol). |
| c) RNA still bound to RNeasy Mini spin column membrane | Repeat RNA elution but incubate the RNeasy Mini spin column on the benchtop for 10 min with RNase-free water before centrifuging. |

Comments and suggestions

- d) Ethanol carryover
- During the second wash with Buffer RPE (step 17), be sure to dry the RNeasy Mini spin column membrane by centrifuging at $\geq 8000 \times g$ ($\geq 10,000$ rpm) for 2 minutes at 15–25°C. After centrifugation, carefully remove the column from the collection tube so that the column does not contact the flow-through. Otherwise, carryover of ethanol will occur.
- To eliminate any chance of possible ethanol carryover, place the RNeasy Mini spin column in a new 2 ml collection tube and perform the optional 1-minute centrifugation step as described in step 18 of the protocol.

Low or no recovery of RNA

- RNase-free water incorrectly dispensed
- Add RNase-free water to the center of the RNeasy Mini spin column membrane to ensure that the membrane is completely covered.

Low A_{260}/A_{280} value

- Water used to dilute RNA for A_{260}/A_{280} measurement
- Use 10 mM Tris-Cl, pH 7.5, not RNase-free water, to dilute the sample before measuring purity (s, page 25).

RNA degraded

- a) Inappropriate handling of starting material
- For optimal results, ensure that tissue starting material samples are properly stabilized and stored in RNAprotect TissueReagent (for details, see the *RNAprotect Handbook*).
- For frozen tissue samples, ensure that they were flash-frozen immediately in liquid nitrogen and properly stored at –90°C to –65°C. Perform the RNeasy procedure quickly, especially the first few steps.
- See “Appendix A: General Remarks on Handling RNA”, page 25, and “Handling and storing starting material”, page 12.
- b) RNase contamination
- Although all RNeasy buffers have been tested and are guaranteed RNase-free, RNases can be introduced during use. Be certain not to introduce any RNases during the RNeasy procedure or later handling. See Appendix A, page 25, and “Handling and storing starting material”.
- Do not put RNA samples into a vacuum dryer that has been used in DNA preparation where RNases may have been used.

DNA contamination in downstream experiments

- No DNase treatment
- Perform on-column DNase digestion using the RNase-Free DNase Set, as described in the protocol. Alternatively, perform DNase digestion after RNA purification. See Appendix B, page 28.
- For real-time, two-step RT-PCR experiments, carry out the RT step using the QuantiNova® Reverse Transcription Kit (cat. no. 205410), which provides cDNA synthesis with integrated removal of genomic DNA contamination.

Comments and suggestions

RNA does not perform well in downstream experiments

- a) Salt carryover during elution Ensure that Buffer RPE is at 15–25°C.
- b) Ethanol carryover During the second wash with Buffer RPE (step 17), be sure to dry the RNeasy Mini spin column membrane by centrifuging at 8000 × g (10,000 rpm) for 2 min at 15–25°C. After centrifugation, carefully remove the column from the collection tube so that the column does not contact the flow-through. Otherwise, carryover of ethanol will occur.

To eliminate any chance of possible ethanol carryover, place the RNeasy Mini spin column in a new 2 ml collection tube and perform the optional 1-minute centrifugation step as described in step 18 of the protocol.

Appendix A: General Remarks on Handling RNA

Handling RNA

Ribonucleases (RNases) are very stable and active enzymes that generally do not require cofactors to function. Since RNases are difficult to inactivate and even minute amounts are sufficient to destroy RNA, do not use any plasticware or glassware without first eliminating possible RNase contamination. Great care should be taken to avoid inadvertently introducing RNases into the RNA sample during or after the purification procedure. To create and maintain an RNase-free environment, the following precautions must be taken during pretreatment and use of disposable and nondisposable vessels and solutions while working with RNA.

General handling

Proper microbiological, aseptic technique should always be used when working with RNA. Hands and dust particles may carry bacteria and molds and are the most common sources of RNase contamination. Always wear latex or vinyl gloves while handling reagents and RNA samples to prevent RNase contamination from the surface of the skin or from dusty laboratory equipment. Change gloves frequently and keep tubes closed whenever possible. Keep purified RNA on ice when aliquots are pipetted for downstream applications. To remove RNase contamination from bench surfaces, nondisposable plasticware and laboratory equipment (e.g., pipets and electrophoresis tanks), use general laboratory reagents. To decontaminate plasticware, rinse with 0.1 M NaOH, 1 mM EDTA,* followed by RNase-free water (see "Solutions", page 26), or rinse with chloroform* if the plasticware is chloroform-resistant. To decontaminate electrophoresis tanks, clean with detergent (e.g., 0.5% SDS),* rinse with RNase-free water, then rinse with ethanol (if the tanks are ethanol resistant) and allow to dry.

* When working with chemicals, always wear a suitable lab coat, disposable gloves and protective goggles. For more information, consult the appropriate safety data sheets (SDSs), available from the product supplier.

Disposable plasticware

The use of sterile, disposable polypropylene tubes is recommended throughout the procedure. These tubes are generally RNase-free and do not require pretreatment to inactivate RNases.* When working with chemicals, always wear a suitable lab coat, disposable gloves and protective goggles. For more information, consult the appropriate safety data sheets (SDSs), available from the product supplier. Glassware should be treated before use to ensure that it is RNase-free. Glassware used for RNA work should be cleaned with a detergent,* thoroughly rinsed and oven baked at 240°C for at least 4 hours (overnight, if more convenient) before use. Autoclaving alone will not fully inactivate many RNases. Alternatively, glassware can be treated with diethyl pyrocarbonate (DEPC)*, as described in “Solutions” below.

Solutions

Solutions (water and other solutions) should be treated with 0.1% DEPC. DEPC is a strong, but not absolute, inhibitor of RNases. It is commonly used at a concentration of 0.1% to inactivate RNases on glass or plasticware or to create RNase-free solutions and water. DEPC inactivates RNases by covalent modification. Add 0.1 ml DEPC to 100 ml of the solution to be treated and shake vigorously to bring the DEPC into solution. Let the solution incubate for 12 hours at 37°C. Autoclave for 15 minutes to remove any trace of DEPC. DEPC will react with primary amines and cannot be used directly to treat Tris* buffers. DEPC is highly unstable in the presence of Tris buffers and decomposes rapidly into ethanol and CO₂. When preparing Tris buffers, treat water with DEPC first, and then dissolve Tris to make the appropriate buffer. Trace amounts of DEPC will modify purine residues in RNA by carbethoxylation. Carbethoxylated RNA is translated with very low efficiency in cell-free systems. However, its ability to form DNA:RNA or RNA:RNA hybrids is not seriously affected unless a large fraction of the purine residues has been modified. Residual DEPC must always be eliminated from solutions or vessels by autoclaving or heating to 100°C for 15 minutes.

* When working with chemicals, always wear a suitable lab coat, disposable gloves and protective goggles. For more information, consult the appropriate safety data sheets (SDSs), available from the product supplier.

Note: RNeasy buffers are guaranteed RNase-free without using DEPC treatment and are therefore free of any DEPC contamination.

Appendix B: Storage, Quantification and Determination of Quality of RNA

Storage of RNA

Purified RNA may be stored at -70°C to -15°C in RNase-free water. Under these conditions, no degradation of RNA is detectable after 1 year.

Quantification of RNA

The concentration of RNA should be determined by measuring the absorbance at 260 nm (A_{260}) in a spectrophotometer (see "Spectrophotometric quantification of RNA" below). For small amounts of RNA, however, it may be difficult to determine amounts photometrically. Small amounts of RNA can be quantified using quantitative RT-PCR or fluorometric quantification.

Spectrophotometric quantification of RNA

Using the QIAxpert UV/VIS Spectrophotometer for microvolume analysis

To determine the concentration of your RNA sample purified with RNeasy QIAGEN kit, use the corresponding RNeasy App on the QIAxpert. For more information, see the QIAxpert product page (www.qiagen.com/qiaexpert-system).

Using a standard spectrophotometer

To ensure significance, A_{260} readings should be greater than 0.15. An absorbance of 1 unit at 260 nm corresponds to 44 μg of RNA per ml ($A_{260} = 1 \rightarrow 4 \mu\text{g/ml}$). This relation is valid only for measurements at a neutral pH. Therefore, if it is necessary to dilute the RNA sample,

this should be done in a buffer with neutral pH.* As discussed below (see “Purity of RNA”, page 29), the ratio between the absorbance values at 260 and 280 nm gives an estimate of RNA purity. When measuring RNA samples, be certain that cuvettes are RNase-free, especially if the RNA is to be recovered after spectrophotometry. This can be accomplished by washing cuvettes with 0.1 M NaOH, 1 mM EDTA,* followed by washing with RNase-free water (see “Solutions”, page 26). Use the buffer in which the RNA is diluted to zero the spectrophotometer. An example of the calculation involved in RNA quantification is shown below:

Volume of RNA sample	= 100 μ l
Dilution	= 10 μ l of RNA sample + 490 μ l of 10 mM Tris-Cl,* pH 7.0 (1/50 dilution)

Measure absorbance of diluted sample in a 1 ml cuvette (RNase-free)

A_{260}	= 0.2
Concentration of RNA sample	= 44 μ g/ml $\times A_{260}$ \times dilution factor = 44 μ g/ml \times 0.2 \times 50 = 440 μ g/ml

Total amount	= concentration \times volume in milliliters = 440 μ g/ml \times 0.1 ml = 44 μ g of RNA
--------------	---

Purity of RNA

The assessment of RNA purity will be performed routinely, when using the QIAxpert with the corresponding RNeasy App. See the QIAxpert user manual for more information (www.qiagen.com/qiexpert-system/user manual)

* When working with chemicals, always wear a suitable lab coat, disposable gloves and protective goggles. For more information, consult the appropriate safety data sheets (SDSs), available from the product supplier.

For standard photometric measurements, the ratio of the readings at 260 nm and 280 nm (A_{260}/A_{280}) provides an estimate of the purity of RNA with respect to contaminants, such as protein, that absorb in the UV spectrum. However, the A_{260}/A_{280} ratio is influenced considerably by pH. Since water is not buffered, the pH and the resulting A_{260}/A_{280} ratio can vary greatly when using pure water. Lower pH results in a lower A_{260}/A_{280} ratio and reduced sensitivity to protein contamination.* For accurate values, we recommend measuring absorbance in 10 mM Tris-Cl, pH 7.5. Pure RNA has an A_{260}/A_{280} ratio of 1.9–2.1† in 10 mM Tris-Cl, pH 7.5. Always be sure to calibrate the spectrophotometer with the same solution used for dilution. For determination of RNA concentration, however, we recommend dilution of the sample in a buffer with neutral pH since the relationship between absorbance and concentration (A_{260} reading of 1 = 44 µg/ml RNA) is based on an extinction coefficient calculated for RNA at neutral pH (see “Spectrophotometric quantification of RNA”, page 28).

DNA contamination

No currently available purification method can guarantee that RNA is completely free of DNA, even when it is not visible on an agarose gel. RNeasy Kits will, however, remove the vast majority of cellular DNA. gDNA Eliminator Solution helps to further reduce genomic DNA contamination; however, trace amounts of genomic DNA may still remain, depending on the amount and nature of the sample. For analysis of very low abundance targets, any interference by residual DNA contamination can be detected by performing real-time RT-PCR control experiments in which no reverse transcriptase is added prior to the PCR step.

To prevent any interference by DNA in real-time RT-PCR applications, such as with Applied Biosystems® and Rotor-Gene® instruments, we recommend designing primers that anneal at intron splice junctions so that genomic DNA will not be amplified. QuantiNova Primer Assays from QIAGEN are designed for SYBR® Green-based real-time RT-PCR analysis of RNA

* Wilfinger, W.W., Mackey, M., and Chomczynski, P. (1997) Effect of pH and ionic strength on the spectrophotometric assessment of nucleic acid purity. *BioTechniques* **22**, 474.

† Values up to 2.3 are routinely obtained for pure RNA (in 10 mM Tris-Cl, pH 7.5) with some spectrophotometers.

sequences (without detection of genomic DNA) where possible (see www.qiagen.com/GeneGlobe). For real-time RT-PCR assays where amplification of genomic DNA cannot be avoided, we recommend using the QuantiNova Reverse Transcription Kit for reverse transcription. The kit integrates fast cDNA synthesis with rapid removal of genomic DNA contamination (see ordering information, page 34).

Integrity of RNA

The integrity and size distribution of total RNA purified with RNeasy Plus Universal Kits can be checked by denaturing agarose gel electrophoresis and ethidium bromide staining* or by using the QIAxcel system or Agilent 2100 Bioanalyzer. Ribosomal RNAs should appear as sharp bands or peaks. The apparent ratio of 28S rRNA to 18S rRNA should be approximately 2:1. If the ribosomal bands or peaks of a specific sample are not sharp, but appear as a smear towards smaller sized RNAs, it is likely that the sample suffered major degradation either before or during RNA purification. As a useful measure of RNA integrity, the QIAxcel Advanced® system and the Agilent 2100 Bioanalyzer provide an RNA integrity score (RIS) and an RNA integrity number (RIN), respectively. Ideally, the value should be close to 10, but in many cases (particularly with tissue samples), RNA quality is greatly influenced by how well the original sample was preserved.

* When working with chemicals, always wear a suitable lab coat, disposable gloves and protective goggles. For more information, consult the appropriate safety data sheets (SDSs), available from the product supplier.

Appendix C: DNase Digestion of RNA Eluates using the RNase-Free DNase Set

As an alternative to on-column DNase digestion (steps 12–15), DNase digestion of RNA eluates can be performed using The RNase-Free DNase Set (cat. no. 79254) instead. For samples with high DNA content, we recommend DNase digestion of RNA eluates, as it is more efficient than on-column DNase digestion.

Important points before starting

- **Do not vortex the reconstituted DNase I.** DNase I is especially sensitive to physical denaturation. Mixing should only be carried out by gently inverting the tube.

Things to do before starting

- Prepare DNase I stock solution before using the RNase-Free DNase Set for the first time. Dissolve the lyophilized DNase I (1500 Kunitz units) in 550 µl of the RNase-free water provided. To avoid loss of DNase I, do not open the vial. Inject RNase-free water into the vial using an RNase-free needle and syringe. Mix gently by inverting the vial. Do not vortex.
- For long-term storage of DNase I, remove the stock solution from the glass vial, divide it into single-use aliquots, and store at –30°C to –15°C for up to 9 months. Thawed aliquots can be stored at 2–8°C for up to 6 weeks. Do not refreeze the aliquots after thawing.

Procedure

1. Purify RNA according to the standard protocol (page 15), but without performing the on-column DNase digestion described in steps 12–14 (instead, perform the optional wash with Buffer RW1 described in step 12).

-
2. Mix the following in a microcentrifuge tube:

87.5 µl RNA eluate

10 µl Buffer RDD

2.5 µl DNase I stock solution

3. Make the volume up to 100 µl with RNase-free water.

The reaction volumes can be doubled if necessary (to 200 µl final volume).

4. Incubate on the benchtop (15–25°C) for 10 min.

5. Clean up the RNA using the RNeasy Mini Kit (cat. no. 74104).

Ordering Information

Product	Contents	Cat. no.
RNeasy Fibrous Tissue Mini Kit (50)	50 RNeasy Mini Spin Columns, Collection Tubes, Proteinase K, RNase-Free DNase I, RNase-Free Reagents and Buffers	74704
QIAcube Connect — for fully automated nucleic acid extraction with QIAGEN spin-column kits		
QIAcube Connect*	Instrument, connectivity package, 1-year warranty on parts and labor	Inquire
Starter Pack, QIAcube	Filter-tips, 200 µl (1024), 1000 µl filter-tips (1024), 30 ml reagent bottles (12), rotor adapters (240); elution tubes (240), rotor adapter holder	990395
Rotor Adapters (10 x 24)	For 240 preps: 240 Disposable Rotor Adapters and 240 Elution Tubes (1.5 ml); for use with the QIAcube	990394
Accessories		
Allprotect Tissue Reagent (100 ml)	For stabilization of DNA, RNA and protein in 50 x 200 mg tissue samples: 100 ml Allprotect Tissue Reagent, Allprotect Reagent Pump	76405
RNAprotect Tissue Reagent (50 ml)	50 ml RNAprotect Tissue Reagent for stabilization of RNA in 25 x 200 mg tissue samples	76104
RNAprotect Tissue Reagent (250 ml)	250 ml RNAprotect Tissue Reagent for stabilization of RNA in 125 x 200 mg tissue samples	76106
RNAprotect Tissue Tubes (50 x 1.5 ml)	For stabilization of RNA in 50 x 50 mg tissue samples: 50 screw-top tubes containing 1.5 ml RNAprotect Tissue Reagent each	76154

Product	Contents	Cat. no.
RNAprotect Tissue Tubes (20 x 5 ml)	For stabilization of RNA in 20 x 500 mg tissue samples: 20 screw-top tubes containing 5 ml RNAprotect Tissue Reagent each	76163
QuantiNova Reverse Transcription Kit (200)	For 200 x 20 µl reactions: 4 x 100 µl 8x gDNA Removal Mix, 4 x 50 µl Reverse Transcription Enzyme, 4 x 200 µl Reverse Transcription Mix (containing RT primers), 4 x 100 µl Internal Control RNA, 4 x 1.9 ml RNase-Free Water	205413
TissueRuptor II	Handheld rotor–stator homogenizer, 5 TissueRuptor Disposable Probes	Inquire
TissueLyser II	Bead mill; requires the TissueLyser Adapter Set 2 x 24 or TissueLyser Adapter Set 2 x 96 (available separately)	Inquire
TissueRuptor Disposable Probes (25)	25 nonsterile plastic disposable probes for use with the TissueRuptor II	990890
TissueLyser Adapter Set 2 x 24	2 sets of Adapter Plates and 2 racks for use with 2 ml microcentrifuge tubes on the TissueLyser II	69982
TissueLyser Adapter Set 2 x 96	2 sets of Adapter Plates for use with Collection Microtubes (racked) on the TissueLyser II	69984
TissueLyser Single-Bead Dispenser, 5 mm	For dispensing individual beads (5 mm diameter)	69965

Product	Contents	Cat. no.
Stainless Steel Beads, 5 mm (200)	Stainless Steel Beads, suitable for use with the TissueLyser system	69989
RNase-Free DNase Set (50)	1500 Kunitz units RNase-free DNase I, RNase-free Buffer RDD and RNase-free water for 50 RNA minipreps	79254

* All QIAcube Connect instruments are provided with a region-specific connectivity package, including tablet and equipment necessary to connect to the local network. Further, QIAGEN offers comprehensive instrument service products, including service agreements, installation, introductory training and preventive subscription. Contact your local sales representative to learn about your options.

For up-to-date licensing information and product-specific disclaimers, see the respective QIAGEN kit handbook or user manual. QIAGEN kit handbooks and user manuals are available at www.qiagen.com or can be requested from QIAGEN Technical Services or your local distributor.

Document Revision History

Date	Changes
October 2010	Initial release.
December 2014	Changes to comply with GHS regulation, throughout the document.
January 2018	Removal of RNeasy Fibrous Midi Kit (cat. no. 75742), including associated protocols, general kit information (Table 1 and Table 2) and ordering information. Update into Sample-to-Insight branding and edit into revised style.
February 2019	Changed numbering of steps in the protocol. Added information about the QIAxcel. Updated text and ordering information for QIAcube Connect. Corrected product name in “Integrity of RNA” and step numbers in Appendix C. Updated format and ordering information. Corrected typographical errors.
November 2020	Updated branding of RNA protection products.

Notes

Notes

Limited License Agreement for RNeasy Fibrous Tissue Mini Kit

Use of this product signifies the agreement of any purchaser or user of the product to the following terms:

1. The product may be used solely in accordance with the protocols provided with the product and this handbook and for use with components contained in the kit only. QIAGEN grants no license under any of its intellectual property to use or incorporate the enclosed components of this kit with any components not included within this kit except as described in the protocols provided with the product, this handbook, and additional protocols available at www.qiagen.com. Some of these additional protocols have been provided by QIAGEN users for QIAGEN users. These protocols have not been thoroughly tested or optimized by QIAGEN. QIAGEN neither guarantees them nor warrants that they do not infringe the rights of third-parties.
2. Other than expressly stated licenses, QIAGEN makes no warranty that this kit and/or its use(s) do not infringe the rights of third-parties.
3. This kit and its components are licensed for one-time use and may not be reused, refurbished, or resold.
4. QIAGEN specifically disclaims any other licenses, expressed or implied other than those expressly stated.
5. The purchaser and user of the kit agree not to take or permit anyone else to take any steps that could lead to or facilitate any acts prohibited above. QIAGEN may enforce the prohibitions of this Limited License Agreement in any Court, and shall recover all its investigative and Court costs, including attorney fees, in any action to enforce this Limited License Agreement or any of its intellectual property rights relating to the kit and/or its components.

For updated license terms, see www.qiagen.com.

Trademarks: QIAGEN®, Sample to Insight®, QIAcube®, QIAxcel®, QIAxper®, AllProtect®, QuantiNova®, RNeasy®, Rotor-Gene®, TissueRuptor® (QIAGEN Group); Agilent® (Agilent Technologies, Inc.); Applied Biosystems®, SYBR® (Thermo Fisher Scientific Inc.). Registered names, trademarks, etc. used in this document, even when not specifically marked as such, are not to be considered unprotected by law.

HB-0485-006 © 2020 QIAGEN, all rights reserved.

Ordering www.qiagen.com/shop | Technical Support support.qiagen.com | Website www.qiagen.com