



July 2023

# QIAGEN<sup>®</sup> Plasmid Purification Handbook

QIAGEN Plasmid Mini, Midi, Maxi, Mega, and  
Giga Kits

For purification of ultrapure, transfection-grade  
plasmid DNA

# Contents

Kit Contents.....	3
Shipping and Storage .....	5
Intended Use .....	5
Safety Information.....	6
Quality Control.....	6
Introduction .....	7
Principle and procedure .....	7
Equipment and Reagents to Be Supplied by User .....	9
Important Notes.....	10
Protocol: Plasmid or Cosmid DNA Purification Using QIAGEN Plasmid Mini Kit.....	18
Protocol: Plasmid or Cosmid DNA Purification Using QIAGEN Plasmid Midi and Maxi Kits .....	24
Protocol: Plasmid or Cosmid DNA Purification Using QIAGEN Plasmid Mega and Giga Kits .....	31
Protocol: Very Low-Copy Plasmid/Cosmid Purification Using QIAGEN-tip 100 or QIAGEN-tip 500 .....	40
Troubleshooting Guide .....	48
Appendix A: Agarose Gel Analysis of the Purification Procedure.....	54
Appendix B: Composition of Buffers.....	58
Ordering Information .....	61
Document Revision History .....	66

# Kit Contents

<b>QIAGEN Plasmid Kit</b>	<b>Mini (25)</b>	<b>Mini (100)</b>	<b>Midi (25)</b>	<b>Midi (100)</b>	<b>Maxi (10)</b>	<b>Maxi (25)</b>	<b>Maxi (100)</b>
<b>Catalog no.</b>	<b>12123</b>	<b>12125</b>	<b>12143</b>	<b>12145</b>	<b>12162</b>	<b>12163</b>	<b>12165</b>
QIAGEN-tip 20	25	100	–	–	–	–	–
QIAGEN-tip 100	–	–	25	100	–	–	–
QIAGEN-tip 500	–	–	–	–	10	25	4 x 25
Buffer P1	20 mL	2 x 20 mL	110 mL	500 mL	110 mL	2 x 150 mL	8 x 150 mL
Buffer P2	20 mL	2 x 20 mL	110 mL	500 mL	110 mL	2 x 150 mL	8 x 150 mL
Buffer P3	20 mL	2 x 20 mL	110 mL	500 mL	110 mL	2 x 150 mL	8 x 150 mL
Buffer QBT	60 mL	2 x 60 mL	2 x 60 mL	500 mL	2 x 60 mL	2 x 200 mL	8 x 200 mL
Buffer QC	2 x 60 mL	2 x 240 mL	3 x 205 mL	5 x 500 mL	3 x 240 mL	4 x 500 mL	16 x 500 mL
Buffer QF	30 mL	140 mL	200 mL	4 x 140 mL	200 mL	510 mL	4 x 510 mL
RNase A*	2 mg	2 x 2 mg	11 mg	50 mg	11 mg	2 x 15 mg	8 x 15 mg
LyseBlue®	20 µL	2 x 20 µL	110 µL	500 µL	110 µL	2 x 150 µL	8 x 150 µL
Quick-Start Protocol	1	1	1	1	1	1	1

\* Provided in a 10 mg/mL or 100 mg/mL solution.

<b>QIAGEN Plasmid Kit</b>	<b>Mega (5)</b>	<b>Mega (25)</b>	<b>Giga (5)</b>	<b>Plasmid Buffer Set</b>
<b>Catalog no.</b>	<b>12181</b>	<b>12183</b>	<b>12191</b>	<b>19046</b>
QIAGEN-tip 2500	5	25	–	–
QIAGEN-tip 10000	–	–	5	–
Buffer P1	2 x 150 mL	3 x 500 mL	3 x 250 mL	110 mL
Buffer P2	2 x 150 mL	3 x 500 mL	3 x 250 mL	110 mL
Buffer P3	2 x 150 mL	3 x 500 mL	3 x 250 mL	110 mL
Buffer QBT	200 mL	2 x 500 mL	2 x 200 mL	2 x 60 mL
Buffer QC	5 x 240 mL	11 x 500 mL	7 x 500 mL	3 x 240 mL
Buffer QF	200 mL	2 x 510 mL	510 mL	2 x 85 mL
RNase A*	2 x 15 mg	3 x 50 mg	3 x 25 mg	11 mg
LyseBlue	2 x 150 µL	3 x 500 µL	3 x 250 µL	110 µL
Quick-Start Protocol	1	1	1	1

\* Provided in a 10 mg/mL or 100 mg/mL solution.

## Shipping and Storage

QIAGEN tips should be stored dry and at room temperature (15–25°C). Under these conditions, the components are stable for 2 years without showing any reduction in performance and quality, unless otherwise indicated on the label.

The QIAGEN Plasmid Kits should be stored at room temperature. After adding RNase A, Buffer P1 should be stored at 2–8°C. Under these conditions, the components are stable for 6 months without showing any reduction in performance and quality.

Other buffers and RNase A stock solution can be stored for 2 years at room temperature.

## Intended Use

The QIAGEN Plasmid Kits are intended for molecular biology applications. These products are not intended for the diagnosis, prevention, or treatment of a disease.

All due care and attention should be exercised in the handling of the products. We recommend all users of QIAGEN products to adhere to the NIH guidelines that have been developed for recombinant DNA experiments, or to other applicable guidelines.

## Safety Information

When working with chemicals, always wear a suitable lab coat, disposable gloves, and protective goggles. For more information, please consult the appropriate safety data sheets (SDSs). These are available online in convenient and compact PDF format at [www.qiagen.com/safety](http://www.qiagen.com/safety), where you can find, view, and print the SDS for each QIAGEN kit and kit component.

## Quality Control

In accordance with QIAGEN's ISO-certified Quality Management System, each lot of the QIAGEN Plasmid Kit is tested against predetermined specifications to ensure consistent product quality.

# Introduction

The QIAGEN Plasmid Purification Kits are based on the remarkable selectivity of patented QIAGEN resin, allowing purification of ultrapure supercoiled plasmid DNA with high yields.

Anion-exchange–based QIAGEN-tips yield transfection-grade DNA, which is highly suited for use in a broad variety of demanding applications such as transfection, *in vitro* transcription and translation, and enzymatic modifications. QIAGEN offers the most comprehensive portfolio of tailored plasmid purification kits for any scale, throughput, or downstream application. Select the optimum kit for your requirements by visiting our online selection guide at [www.qiagen.com/plasmidselectionguide](http://www.qiagen.com/plasmidselectionguide). For transfection, QIAGEN also offers the advanced PolyFect<sup>®</sup>, SuperFect<sup>®</sup>, and Effectene<sup>®</sup> transfection reagents. These reagents, combined with the high-quality plasmid DNA obtained from QIAGEN, QIAfilter, HiSpeed<sup>®</sup>, and EndoFree<sup>®</sup> Plasmid Kits, provide optimal transfection results (see “Ordering Information”, page 61).

## Principle and procedure

QIAGEN plasmid purification protocols are based on a modified alkaline lysis procedure, followed by binding of plasmid DNA to QIAGEN resin under appropriate low-salt and pH conditions. RNA, proteins, dyes, and low-molecular–weight impurities are removed by a medium-salt wash. Plasmid DNA is eluted in a high-salt buffer and then concentrated and desalted by isopropanol precipitation.

Each disposable QIAGEN-tip packed with QIAGEN resin is designed to operate by gravity flow, reducing the amount of hands-on time required for the purification procedure.

## QIAGEN Plasmid Kits

Pelleted bacteria



Alkaline lysate



Clear lysate  
by centrifugation



Bind DNA



Wash



Elute



Isopropanol precipitate



Ultrapure plasmid DNA

# Equipment and Reagents to Be Supplied by User

When working with chemicals, always wear a suitable lab coat, disposable gloves, and protective goggles. For more information, consult the appropriate safety data sheets (SDSs), available from the product supplier.

## For all protocols

- Standard microbiological equipment for growing and harvesting bacteria (e.g., inoculating loop, culture tubes and flasks, 37°C shaking incubator, and centrifuge with rotor and tubes or bottles for harvesting cells)
- QIArack (cat. no. 19015) or equivalent holder (see “Setup of QIAGEN-tips”, page 15)
- Ice
- Isopropanol
- Ethanol, 70%
- Plasmid resuspension buffer (e.g., TE buffer, pH 8.0, or Tris-Cl, pH 8.5)

## For the QIAGEN Plasmid Mini Kit protocol

- Microcentrifuge
- 1.5 mL or 2 mL microcentrifuge tubes

## For QIAGEN Plasmid Midi, Maxi, Mega, and Giga Kit protocols

- Centrifugation tubes or vessels with suitable capacity for the volumes specified in the appropriate protocol
- Refrigerated centrifuge capable of  $\geq 20,000 \times g$  with a rotor for the appropriate centrifuge tubes or bottles

# Important Notes

Please take a few moments to read this handbook carefully before beginning the DNA preparation. If QIAGEN Plasmid Purification Kits are new to you, please visit our plasmid resource page at [www.qiagen.com/goto/plasmidinfo](http://www.qiagen.com/goto/plasmidinfo). Also be sure to read and follow the appropriate detailed protocol.

## Plasmid size

Plasmids up to approximately 150 kb can be purified using QIAGEN plasmid purification protocols. Constructs larger than 45–50 kb, however, may exhibit somewhat reduced elution efficiencies. Prewarming the elution buffer to 65°C may help to increase the yield of large plasmids. For the isolation of large cosmid and plasmid DNA constructs, the QIAGEN Large-Construct Kit is available (see “Ordering Information”, page 61).

## Plasmid/cosmid copy number

Plasmids and cosmids vary in copy number, depending on the origin of replication they contain, their size, and the size of insert. The protocols in this handbook are grouped according to the copy number of the plasmid or cosmid to be purified.

High- and low-copy plasmids and cosmids should be purified using one of these protocols:

- “Protocol: Plasmid or Cosmid DNA Purification Using QIAGEN Plasmid Mini Kit”, page 18
- “Protocol: Plasmid or Cosmid DNA Purification Using QIAGEN Plasmid Midi and Maxi Kits”, page 24
- “Protocol: Plasmid or Cosmid DNA Purification Using QIAGEN Plasmid Mega and Giga Kits”, page 31

Very low-copy plasmids and very low-copy cosmids (<10 copies per cell) should be purified using "Protocol: Very Low-Copy Plasmid/Cosmid Purification Using QIAGEN-tip 100 or QIAGEN-tip 500", page 40, which uses extremely large culture volumes to obtain good yields.

For more details, visit our plasmid resource page at [www.qiagen.com/goto/plasmidinfo](http://www.qiagen.com/goto/plasmidinfo).

## Host strains

The strain used to propagate a plasmid can have a substantial influence on quality of the purified DNA. Host strains such as DH1, DH5<sup>®</sup>α, and C600 yield high-quality DNA with QIAGEN protocols. The slower-growing strain XL1-Blue also yields DNA of very high quality.

Strain HB101 and its derivatives, such as TG1 and the JM100 series, contain large amounts of carbohydrates that are released during lysis and can inhibit enzyme activities if not completely removed. In addition, some strains, such as JM101, JM110, and HB101, have high levels of endonuclease activity and yield DNA of lower quality. If the quality of purified DNA is not as expected, a change of host strain should be considered. If difficulty is encountered with strains such as TG1 and Top10F, we recommend either reducing the amount of culture volume or doubling the volumes of Buffers P1, P2, and P3 to improve the ratio of biomass to lysis buffers for optimized lysis conditions.

**Table 1. Origins of replication and copy numbers of various plasmids and cosmids**

DNA construct	Origin of replication	Copy number	Classification
<b>Plasmids</b>			
pUC vectors	pMB1 *	500–700	High copy
pBluescript® vectors	ColE1	300–500	High copy
pGEM® vectors	pMB1 *	300–400	High copy
pTZ vectors	pMB1 *	>1000	High copy
pBR322 and derivatives	pMB1 *	15–20	Low copy
pACYC and derivatives	p15A	10–12	Low copy
pSC101 and derivatives	pSC101	~5	Very low copy
<b>Cosmids</b>			
SuperCos	pMB1	10–20	Low copy
pWE15	ColE1	10–20	Low copy

\* The pMB1 origin of replication is closely related to that of ColE1 and falls in the same incompatibility group. The high-copy plasmids listed here contain mutated versions of this origin.

## Culture media

QIAGEN plasmid purification protocols are optimized for use with cultures grown in standard Luria Bertani (LB) medium to a cell density of approximately  $3\text{--}4 \times 10^9$  cells/mL, which typically corresponds to a pellet wet weight of approximately 3 g/L medium. Please note that a number of slightly different LB culture broths, containing different concentrations of NaCl, are commonly used. We recommend growing cultures in LB medium containing 10 g NaCl per liter (Table 2) to obtain the highest plasmid yields.

Rich media are not recommended for plasmid preparation with QIAGEN-tips. If rich media must be used, growth time must be optimized and culture volumes reduced. For more details, visit our plasmid resource page at [www.qiagen.com/goto/plasmidinfo](http://www.qiagen.com/goto/plasmidinfo).

**Table 2. Composition of Luria Bertani (LB)\* medium**

Contents	Per liter
Tryptone	10 g
Yeast extract	5 g
NaCl	10 g

\* See Appendix B, page 58, for preparation of LB medium.

## Culture volume

Do not exceed the maximum recommended culture volumes given at the beginning of each protocol (and on the card inside the back cover of this handbook). Using larger culture volumes will lead to an increase in biomass and can affect the efficiency of alkaline lysis, leading to reduced yield and purity of the preparation.

The protocol for the QIAGEN Plasmid Kits is optimized for use with cultures grown in standard LB medium, grown to a cell density of approximately  $3\text{--}4 \times 10^9$  cells per mL. We advise harvesting cultures after approximately 12–16 hours of growth, which typically is the transition from logarithmic into stationary growth phase. It is best to assess the cell density of the culture and, if that is too high, to reduce the culture volumes accordingly or increase the volumes of Buffers P1, P2, and P3. A high ratio of biomass to lysis buffers will result in poor lysis conditions and subsequently low DNA yield and purity. For determination of cell density, calibration of each individual spectrophotometer is required to facilitate accurate conversion of OD<sub>600</sub> measurements into the number of cells per milliliter. This can be achieved by plating serial dilutions of a culture onto LB-agar plates in the absence of antibiotics. The counted colonies are used to calculate the number of cells per milliliter, which is then set in relation to the measured OD<sub>600</sub> values.

## Capacity of QIAGEN-tips

QIAGEN-tips are available in a variety of sizes for preparation of as little as 20 µg or as much as 10 mg plasmid DNA (Figure 1). The maximum plasmid-binding capacities of the QIAGEN-tips 20, 100, 500, 2500, and 10000 are at least 20 µg, 100 µg, 500 µg, 2.5 mg, and 10 mg, respectively. Actual yields will depend on culture volume, culture medium, plasmid copy number, size of insert, and host strain. For more details, visit our plasmid resource page at [www.qiagen.com/goto/plasmidinfo](http://www.qiagen.com/goto/plasmidinfo).

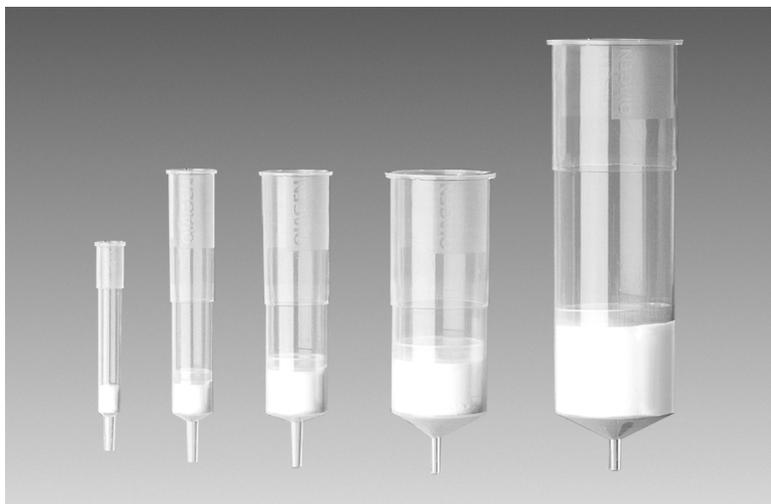
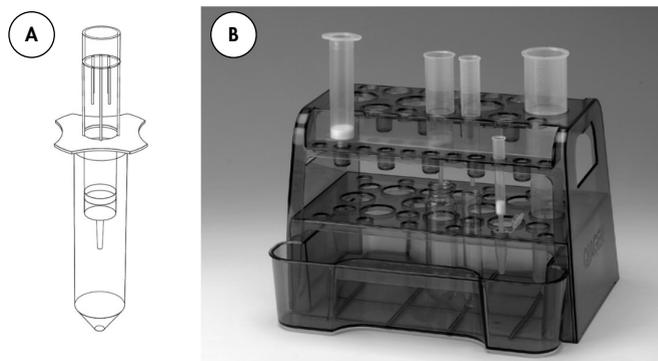


Figure 1. QIAGEN-tip 20 to QIAGEN-tip 10000.

## Setup of QIAGEN-tips

QIAGEN-tips may be held upright in a suitable collection vessel such as a tube or flask, using the tip holders provided with the kits (Figure 2A). Alternatively, the QIAGEN-tips 20, 100, 500, and 2500 may be placed in the QIArack (cat. no. 19015) (Figure 2B).



**Figure 2.** Setup of QIAGEN-tips (A) with tip holder or (B) with the QIArack.

Optional if using the QIAfilter Mega-Giga Cartridge for lysate clearing:



**Figure 3.** The vacuum-operated QIAfilter Mega-Giga Cartridge in use. Note that the bottle is not included in kits.

## Analytical gel analysis

The success of the plasmid purification procedure can be monitored on an analytical gel (Figure 4, page 55). We recommend removing and saving aliquots where indicated during the purification procedure (samples 1–4). If the plasmid DNA is of low yield or low quality, the samples can be analyzed by agarose gel electrophoresis to determine the stage of the purification where the problem occurred (see page 55).

## Convenient stopping points in protocols

For all protocols, the purification procedure can be stopped and continued later by freezing the cell pellets obtained by centrifugation. The frozen cell pellets can be stored at  $-30$  to  $-15^{\circ}\text{C}$  for several weeks. In addition, the DNA eluted from the QIAGEN-tip can be stored overnight at  $2$ – $8^{\circ}\text{C}$ ,\* after which the protocol can be continued.

## Using LyseBlue reagent

LyseBlue is a color indicator that provides visual identification of optimum buffer mixing. This prevents common handling errors that lead to inefficient cell lysis and incomplete precipitation of SDS, genomic DNA, and cell debris. This makes LyseBlue ideal for use by researchers who have not had much experience with plasmid preparations, as well as experienced scientists who want to be assured of maximum product yield.

LyseBlue can be added to the resuspension buffer (Buffer P1) bottle before use. Alternatively, smaller amounts of LyseBlue can be added to aliquots of Buffer P1, enabling single plasmid preparations incorporating visual lysis control to be performed.

\* Longer storage is not recommended.

LyseBlue reagent should be added to Buffer P1 at a ratio of 1:1000 to achieve the required working concentration (e.g., 10  $\mu$ L LyseBlue into 10 mL Buffer P1). Make sufficient LyseBlue/Buffer P1 working solution for the number of plasmid preps being performed.

LyseBlue precipitates after addition into Buffer P1. This precipitate will completely dissolve after addition of Buffer P2. Shake Buffer P1 before use to resuspend LyseBlue particles.

The plasmid preparation procedure is performed as usual. After addition of Buffer P2 to Buffer P1, the color of the suspension changes to blue. Mixing should result in a homogeneously colored suspension. If the suspension contains localized regions of colorless solution or if brownish cell clumps are still visible, continue mixing the solution until a homogeneously colored suspension is achieved.

Upon addition of neutralization buffer (Buffer P3 or Buffer N3), LyseBlue turns colorless. The presence of a homogeneous solution with no traces of blue indicates that SDS from the lysis buffer has been effectively precipitated.

# Protocol: Plasmid or Cosmid DNA Purification Using QIAGEN Plasmid Mini Kit

This protocol is designed for preparation of up to 20 µg of high-copy plasmid or cosmid DNA using the QIAGEN Plasmid Mini Kit. For additional protocols, such as for cosmid, low-copy-number plasmid, BACs, PACs, P1s, and double-stranded M13 replicative form purification, see the recommendations at [www.qiagen.com/goto/plasmidinfo](http://www.qiagen.com/goto/plasmidinfo).

## Important points before starting

- New users are advised to familiarize themselves with the detailed protocol provided in this handbook. In addition, extensive background information is provided on our plasmid resource page, [www.qiagen.com/goto/plasmidinfo](http://www.qiagen.com/goto/plasmidinfo).
- **Optional:** Remove samples at indicated steps to monitor the procedure on an analytical gel (see Appendix A, "Agarose gel analysis", page 55).

## Things to do before starting

- Before use, centrifuge RNase A briefly, and then add into Buffer P1 to obtain a final concentration of 100 µg/mL.
- Check Buffer P2 for SDS precipitation due to low storage temperatures. If necessary, dissolve the SDS by warming to 37°C.
- Prechill Buffer P3 at 4°C.
- **Optional:** Add the provided LyseBlue reagent to Buffer P1 and mix before use. Use 1 vial LyseBlue reagent per bottle Buffer P1 for a final dilution of 1:1000 (e.g., 10 µL LyseBlue into 10 mL Buffer P1). LyseBlue provides visual identification of optimum buffer mixing, thereby preventing the common handling errors that lead to inefficient cell lysis and incomplete precipitation of SDS, genomic DNA, and cell debris. For more details, see "Using LyseBlue reagent" on page 16.

## Procedure

1. Pick a single colony from a freshly streaked selective plate and inoculate a starter culture of 2–5 mL LB medium containing the appropriate selective antibiotic. Incubate for approximately 8 h at 37°C with vigorous shaking (approx. 300 rpm).

Use a tube or flask with a volume of at least 4 times the volume of the culture.

2. Dilute the starter culture 1/500 to 1/1000 into 3 mL selective LB medium. Grow at 37°C for 12–16 h with vigorous shaking (approx. 300 rpm).

Use a flask or vessel with a volume of at least 4 times the volume of the culture. The culture should reach a cell density of approximately  $3\text{--}4 \times 10^9$  cells per milliliter, which typically corresponds to a pellet wet weight of approximately 3 g/L medium.

3. Harvest the bacterial cells by centrifugation at  $6000 \times g$  for 15 min at 4°C.

If you wish to stop the protocol and continue later, freeze the cell pellets at –30 to –15°C.

4. Resuspend the bacterial pellet in 0.3 mL of Buffer P1.

Ensure that RNase A has been added to Buffer P1.

If LyseBlue reagent has been added to Buffer P1, vigorously shake the buffer bottle before use to ensure LyseBlue particles are completely resuspended. The bacteria should be resuspended completely by vortexing or pipetting up and down until no cell clumps remain.

5. Add 0.3 mL of Buffer P2, mix thoroughly by vigorously inverting the sealed tube 4–6 times, and incubate at room temperature for 5 min.

Do not vortex because this will result in shearing of genomic DNA. The lysate should appear viscous. Do not allow the lysis reaction to proceed for more than 5 min. After use, the bottle containing Buffer P2 should be closed immediately to avoid acidification from CO<sub>2</sub> in the air.

If LyseBlue has been added to Buffer P1, the cell suspension will turn blue after addition of Buffer P2. Mixing should result in a homogeneously colored suspension. If the suspension contains localized colorless regions or if brownish cell clumps are still visible, continue mixing the solution until a homogeneously colored suspension is achieved.

6. Add 0.3 mL of chilled Buffer P3, mix immediately and thoroughly by vigorously inverting 4–6 times, and incubate on ice for 5 min.

Precipitation is enhanced by using chilled Buffer P3 and incubating on ice. After addition of Buffer P3, a fluffy white material forms and the lysate becomes less viscous. The precipitated material contains genomic DNA, proteins, cell debris, and KDS. The lysate should be mixed thoroughly to ensure even potassium dodecyl sulphate precipitation. If the mixture still appears viscous, more mixing is required to completely neutralize the solution.

If LyseBlue reagent has been used, the suspension should be mixed until all trace of blue has gone and the suspension is colorless. A homogeneous colorless suspension indicates that the SDS has been effectively precipitated.

7. Centrifuge at maximum speed in a microcentrifuge for 10 min at 4°C. Remove the supernatant containing plasmid DNA promptly.

Before loading the centrifuge, the sample should be mixed again. Centrifugation should be performed at maximum speed in 1.5 mL or 2 mL microcentrifuge tubes (e.g., 10,000–13,000 rpm in a microcentrifuge). Maximum speed corresponds to 14,000–18,000  $\times g$  for most microcentrifuges. After centrifugation, the supernatant should be clear. If the supernatant is not clear, a second, shorter centrifugation should be carried out to avoid applying any suspended or particulate material to the column. Suspended material (which causes the sample to appear turbid) will clog the column and reduce or eliminate flow.

**Optional:** Remove a 50  $\mu\text{L}$  sample from the cleared lysate and save it for an analytical gel (sample 1).

8. Equilibrate a QIAGEN-tip 20 by applying 1 mL Buffer QBT, and allow the column to empty by gravity flow.

Place QIAGEN-tips into a QIArack over the waste tray or use the tip holders provided with each kit (see "Setup of QIAGEN-tips", page 15). Flow of buffer will begin automatically by reduction in surface tension due to the presence of detergent in the equilibration buffer. Allow the QIAGEN-tip to drain completely. QIAGEN-tips can be left unattended because the flow of buffer will stop when the meniscus reaches the upper frit in the column.

9. Apply the supernatant from step 7 to the QIAGEN-tip 20 and allow it to enter the resin by gravity flow.

The supernatant should be loaded onto the QIAGEN-tip promptly. If it is left too long and becomes cloudy due to further precipitation of protein, it must be centrifuged again before loading to prevent clogging of the QIAGEN-tip.

**Optional:** Remove a 50  $\mu$ L sample of the flow-through and save for an analytical gel (sample 2).

10. Wash the QIAGEN-tip 20 with 2 x 2 mL Buffer QC.

Allow Buffer QC to move through the QIAGEN-tip by gravity flow.

**Optional:** Remove a 220  $\mu$ L sample of the combined wash fractions and save for an analytical gel (sample 3).

11. Elute DNA with 0.8 mL Buffer QF.

Collect the eluate in a 1.5 or 2 mL microcentrifuge tubes (not supplied).

**Note:** For constructs larger than 45–50 kb, prewarming the elution buffer to 65°C may help to increase yield.

**Optional:** Remove a 45  $\mu$ L sample of the eluate and save for an analytical gel (sample 4).

12. Precipitate DNA by adding 0.7 volumes (0.56 mL per 0.8 mL of elution volume) of room-temperature isopropanol to the eluted DNA. Mix and centrifuge immediately at  $\geq 15,000 \times g$  for 30 min at 4°C in a microcentrifuge. Carefully decant the supernatant. All solutions should be at room temperature to minimize salt precipitation. Isopropanol pellets have a glassy appearance and may be more difficult to see than the fluffy, salt-containing pellets that result from ethanol precipitation. Marking the outside of the tube before centrifugation allows the pellet to be easily located. Isopropanol pellets are more loosely attached to the side of the tube; take care when removing the supernatant.

13. Wash DNA pellet with 1 mL of 70% ethanol and centrifuge at 15,000  $\times g$  for 10 min. Carefully decant the supernatant without disturbing the pellet.

The 70% ethanol removes precipitated salt and replaces isopropanol with the more volatile ethanol, making the DNA easier to redissolve.

14. Air-dry the pellet for 5–10 min, and redissolve the DNA in a suitable volume of buffer (e.g., TE buffer, pH 8.0, or 10 mM Tris-Cl, pH 8.5).

Redissolve the DNA pellet by rinsing the walls to recover the DNA. Pipetting the DNA up and down to promote resuspension may cause shearing and should be avoided.

Overdrying the pellet will make the DNA difficult to redissolve. DNA dissolves best under slightly alkaline conditions; it does not easily dissolve in acidic buffers.

## Determination of yield

To determine the yield, DNA concentration should be determined by both UV spectrophotometry at 260 nm and quantitative analysis on an agarose gel. For reliable spectrophotometric DNA quantification,  $A_{260}$  readings should lie between 0.1 and 1.0.

## Agarose gel analysis

We recommend removing and saving aliquots during the purification procedure (samples 1–4). If the plasmid DNA is of low yield or quality, the samples can be analyzed by agarose gel electrophoresis to determine the stage of the purification procedure where the problem occurred (see page 55).

# Protocol: Plasmid or Cosmid DNA Purification Using QIAGEN Plasmid Midi and Maxi Kits

This protocol is designed for preparation of up to 100 µg high- or low-copy plasmid or cosmid DNA using the QIAGEN Plasmid Midi Kit, or up to 500 µg using the QIAGEN Plasmid Maxi Kit. For additional protocols, such as for purification of very low-copy plasmids or cosmids of less than 10 copies per cell, see page 40 or visit [www.qiagen.com/goto/plasmidinfo](http://www.qiagen.com/goto/plasmidinfo).

Low-copy plasmids that have been amplified in the presence of chloramphenicol should be treated as high-copy plasmids when choosing the appropriate culture volume.

**Table 3. Maximum recommended culture volumes\***

	QIAGEN-tip 100	QIAGEN-tip 500
High-copy plasmids	25 mL	100 mL
Low-copy plasmids	100 mL	500 mL

\* For the QIAGEN-tip 100, the expected yields are 75–100 µg for high-copy plasmids and 20–100 µg for low-copy plasmids. For the QIAGEN-tip 500, the expected yields are 300–500 µg for high-copy plasmids and 100–500 µg for low-copy plasmids.

## Important points before starting

- New users are advised to familiarize themselves with the detailed protocol provided in this handbook. In addition, extensive background information is provided on our plasmid resource page, [www.qiagen.com/goto/plasmidinfo](http://www.qiagen.com/goto/plasmidinfo).
- If working with low-copy vectors, it may be beneficial to increase the lysis buffer volumes to increase the efficiency of alkaline lysis and, thereby, the DNA yield. In case additional Buffers P1, P2, and P3 are needed, their compositions are provided in Appendix B on page 58. Alternatively, the buffers may be purchased separately (see “Ordering Information”, page 61).

- **Optional:** Remove samples at the indicated steps to monitor the procedure on an analytical gel (see page 55).
- The ▲ symbol denotes values for QIAGEN-tip 100, using the QIAGEN Plasmid Midi Kit; ● denotes values for QIAGEN-tip 500, using the QIAGEN Plasmid Maxi Kit.

## Things to do before starting

- Before use, centrifuge RNase A briefly, and then add into Buffer P1 to obtain a final concentration of 100 µg/mL.
- Check Buffer P2 for SDS precipitation due to low storage temperatures. If necessary, dissolve the SDS by warming to 37°C.
- Prechill Buffer P3 at 4°C.
- **Optional:** Add the provided LyseBlue reagent to Buffer P1 and mix before use. Use 1 vial LyseBlue reagent per bottle of Buffer P1 for a final dilution of 1:1000 (e.g., 10 µL LyseBlue into 10 mL Buffer P1). LyseBlue provides visual identification of optimum buffer mixing, thereby preventing the common handling errors that lead to inefficient cell lysis and incomplete precipitation of SDS, genomic DNA, and cell debris. For more details, see “Using LyseBlue reagent” on page 16.

## Procedure

1. Pick a single colony from a freshly streaked selective plate and inoculate a starter culture of 2–5 mL LB medium containing the appropriate selective antibiotic. Incubate for approximately 8 h at 37°C with vigorous shaking (approx. 300 rpm).  
Use a tube or flask with a volume of at least 4 times the volume of the culture.
2. Dilute the starter culture 1/500 to 1/1000 into selective LB medium.  
For high-copy plasmids, inoculate ▲ 25 mL or ● 100 mL medium with ▲ 25–50 µL or ● 100–200 µL of starter culture.

For low-copy plasmids, inoculate ▲ 100 mL or ● 500 mL medium with ▲ 100–200 µL or ● 250–500 µL of starter culture.

Grow at 37°C for 12–16 h with vigorous shaking (approx. 300 rpm).

Use a flask or vessel with a volume of at least 4 times the volume of the culture. The culture should reach a cell density of approximately  $3\text{--}4 \times 10^9$  cells per milliliter, which typically corresponds to a pellet wet weight of approximately 3 g/L medium.

3. Harvest the bacterial cells by centrifugation at  $6000 \times g$  for 15 min at 4°C.

If you wish to stop the protocol and continue later, freeze the cell pellets at –30 to –15°C.

4. Resuspend the bacterial pellet in ▲ 4 mL or ● 10 mL Buffer P1.

For efficient lysis, it is important to use a vessel that is large enough to allow complete mixing of the lysis buffers. Ensure that RNase A has been added to Buffer P1.

If LyseBlue reagent has been added to Buffer P1, vigorously shake the buffer bottle before use to ensure LyseBlue particles are completely resuspended. The bacteria should be resuspended completely by vortexing or pipetting up and down until no cell clumps remain.

5. Add ▲ 4 mL or ● 10 mL Buffer P2, mix thoroughly by vigorously inverting the sealed tube 4–6 times, and incubate at room temperature for 5 min.

Do not vortex, because this will result in shearing of genomic DNA. The lysate should appear viscous. Do not allow the lysis reaction to proceed for more than 5 min. After use, the bottle containing Buffer P2 should be closed immediately to avoid acidification from CO<sub>2</sub> in the air.

If LyseBlue has been added to Buffer P1, the cell suspension will turn blue after addition of Buffer P2. Mixing should result in a homogeneously colored suspension. If the suspension contains localized colorless regions or if brownish cell clumps are still visible, continue mixing the solution until a homogeneously colored suspension is achieved.

6. Add ▲ 4 mL or ● 10 mL of chilled Buffer P3, mix immediately and thoroughly by vigorously inverting 4–6 times, and incubate on ice for ▲ 15 min or ● 20 min.

Precipitation is enhanced by using chilled Buffer P3 and incubating on ice. After addition of Buffer P3, a fluffy white material forms and the lysate becomes less viscous. The precipitated material contains genomic DNA, proteins, cell debris, and potassium dodecyl sulfate (KDS). The lysate should be mixed thoroughly to ensure even KDS precipitation. If the mixture still appears viscous, more mixing is required to completely neutralize the solution.

If LyseBlue reagent has been used, the suspension should be mixed until all trace of blue has gone and the suspension is colorless. A homogeneous colorless suspension indicates that the SDS has been effectively precipitated.

7. Centrifuge at  $\geq 20,000 \times g$  for 30 min at 4°C. Remove supernatant containing plasmid DNA promptly.

Before loading the centrifuge, the sample should be mixed again. Centrifugation should be performed in non-glass tubes (e.g., polypropylene). After centrifugation the supernatant should be clear.

**Note:** Instead of centrifugation steps 7 and 8, the lysate can be efficiently cleared by filtration using QIAfilter Kits or Cartridges (see [www.qiagen.com/products/discovery-and-translational-research/dna-rna-purification/dna-purification/plasmid-dna/qiafilter-plasmid-kits](http://www.qiagen.com/products/discovery-and-translational-research/dna-rna-purification/dna-purification/plasmid-dna/qiafilter-plasmid-kits)).

8. Centrifuge the supernatant again at  $\geq 20,000 \times g$  for 15 min at 4°C. Remove supernatant containing plasmid DNA promptly.

This second centrifugation step should be carried out to avoid applying suspended or particulate material to the QIAGEN-tip. Suspended material (causing the sample to appear turbid) can clog the QIAGEN-tip and reduce or eliminate gravity flow.

**Optional:** Remove a ▲ 240  $\mu\text{L}$  or ● 120  $\mu\text{L}$  sample from the cleared lysate supernatant and save for an analytical gel (sample 1) to determine whether growth and lysis conditions were optimal.

9. Equilibrate a ▲ QIAGEN-tip 100 or ● QIAGEN-tip 500 by applying ▲ 4 mL or ● 10 mL Buffer QBT, and allow the column to empty by gravity flow.

Flow of buffer will begin automatically by reduction in surface tension due to the presence of detergent in the equilibration buffer. Allow the QIAGEN-tip to drain completely. QIAGEN-tips can be left unattended because the flow of buffer will stop when the meniscus reaches the upper frit in the column.

10. Apply the supernatant from step 8 to the QIAGEN-tip and allow it to enter the resin by gravity flow.

The supernatant should be loaded onto the QIAGEN-tip promptly. If it is left too long and becomes cloudy due to further precipitation of protein, it must be centrifuged again or filtered before loading to prevent clogging of the QIAGEN-tip.

**Optional:** Remove a ▲ 240  $\mu$ L or ● 120  $\mu$ L sample from the flow-through and save for an analytical gel (sample 2) to determine the efficiency of DNA binding to the QIAGEN resin.

11. Wash the QIAGEN-tip with ▲ 2 x 10 mL or ● 2 x 30 mL Buffer QC.

Allow Buffer QC to move through the QIAGEN-tip by gravity flow. The first wash is sufficient to remove contaminants in the majority of plasmid DNA preparations. The second wash is especially necessary when large culture volumes or bacterial strains producing large amounts of carbohydrates are used.

**Optional:** Remove a ▲ 400  $\mu$ L or ● 240  $\mu$ L sample from the combined wash fractions and save for an analytical gel (sample 3).

12. Elute DNA with ▲ 5 mL or ● 15 mL Buffer QF.

Collect the eluate in a ▲ 15 mL or ● 50 mL tube (not supplied). Use of polycarbonate centrifuge tubes is not recommended as polycarbonate is not resistant to the alcohol used in subsequent steps.

**Note:** For constructs larger than 45–50 kb, prewarming the elution buffer to 65°C may help to increase yield.

**Optional:** Remove a ▲ 100  $\mu\text{L}$  or ● 60  $\mu\text{L}$  sample of the eluate and save for an analytical gel (sample 4).

If you wish to stop the protocol and continue later, store the eluate at 4°C. Storage periods longer than overnight are not recommended.

13. Precipitate DNA by adding ▲ 3.5 mL or ● 10.5 mL (0.7 volumes) room-temperature isopropanol to the eluted DNA. Mix and centrifuge immediately at  $\geq 15,000 \times g$  for 30 min at 4°C. Carefully decant the supernatant.

All solutions should be at room temperature to minimize salt precipitation, although centrifugation is carried out at 4°C to prevent overheating of the sample. Alternatively, disposable conical-bottom centrifuge tubes can be used for centrifugation at  $5000 \times g$  for 60 min at 4°C. Isopropanol pellets have a glassy appearance and may be more difficult to see than the fluffy, salt-containing pellets that result from ethanol precipitation. Marking the outside of the tube before centrifugation allows the pellet to be more easily located. Isopropanol pellets are also more loosely attached to the side of the tube, and care should be taken when removing the supernatant.

14. Wash DNA pellet with ▲ 2 mL or ● 5 mL of room-temperature 70% ethanol, and centrifuge at  $\geq 15,000 \times g$  for 10 min. Carefully decant the supernatant without disturbing the pellet.

Alternatively, disposable conical-bottom centrifuge tubes can be used for centrifugation at  $5000 \times g$  for 60 min at 4°C. The 70% ethanol removes precipitated salt and replaces isopropanol with the more volatile ethanol, making the DNA easier to redissolve.

15. Air-dry the pellet for 5–10 min, and redissolve the DNA in a suitable volume of buffer (e.g., TE buffer, pH 8.0, or 10 mM Tris·Cl, pH 8.5).

Redissolve the DNA pellet by rinsing the walls to recover the DNA, especially if glass tubes have been used. Pipetting the DNA up and down to promote resuspension may cause shearing and should be avoided. Overdrying the pellet will make the DNA difficult to redissolve. DNA dissolves best under slightly alkaline conditions; it does not easily dissolve in acidic buffers.

## Determination of yield

To determine the yield, DNA concentration should be determined by both UV spectrophotometry at 260 nm and quantitative analysis on an agarose gel. For reliable spectrophotometric DNA quantification,  $A_{260}$  readings should lie between 0.1 and 1.0.

## Agarose gel analysis

We recommend removing and saving aliquots during the purification procedure (samples 1–4). If the plasmid DNA is of low yield or quality, the samples can be analyzed by agarose gel electrophoresis to determine the stage of the purification procedure where the problem occurred (see page 55).

# Protocol: Plasmid or Cosmid DNA Purification Using QIAGEN Plasmid Mega and Giga Kits

This protocol is designed for preparation of up to 2.5 mg of high- or low-copy plasmid or cosmid DNA using the QIAGEN Plasmid Mega Kit, or up to 10 mg using the QIAGEN Plasmid Giga Kit. For additional protocols, such as for purification of very low-copy plasmids or cosmids <10 copies per cell, see page 40 or visit [www.qiagen.com/goto/plasmidinfo](http://www.qiagen.com/goto/plasmidinfo).

Low-copy plasmids that have been amplified in the presence of chloramphenicol should be treated as high-copy plasmids when choosing the appropriate culture volume.

**Table 4. Maximum recommended culture volumes\***

	QIAGEN-tip 2500	QIAGEN-tip 10000
High-copy plasmids	500 mL (1.5 g pellet wet weight) <sup>†</sup>	2.5 L (7.5 g pellet wet weight) <sup>†</sup>
Low-copy plasmids	2.5 L (7.5 g pellet wet weight) <sup>†</sup>	5 L <sup>††</sup> (15 g pellet wet weight) <sup>††</sup>

\* For the QIAGEN-tip 2500, the expected yields are 1.5–2.5 mg for high-copy plasmids and 0.5–2.5 mg for low-copy plasmids. For the QIAGEN-tip 10000, the expected yields are 7.5–10 mg for high-copy plasmids and 1–5 mg for low-copy plasmids.

<sup>†</sup> On average, a healthy 1 L shaker culture yields a pellet with a wet weight of approximately 3 g. When working with fermentation cultures, however, the pellet wet weight may be significantly higher. Therefore, when using fermented cultures, please refer to the pellet wet weight instead of the recommended culture volumes.

<sup>††</sup> Requires doubled amounts of alkaline lysis buffers.

## Important points before starting

- New users are advised to familiarize themselves with the detailed protocol provided in this handbook. In addition, extensive background information is provided on our plasmid resource page, [www.qiagen.com/goto/plasmidinfo](http://www.qiagen.com/goto/plasmidinfo).

- If working with low-copy vectors, it may be beneficial to increase the lysis buffer volumes to increase the efficiency of alkaline lysis, and thereby the DNA yield. In case additional Buffers P1, P2, and P3 are needed, their compositions are provided in Appendix B, page 58. Alternatively, the buffers may be purchased separately (see “Ordering Information, page 61).
- **Optional:** Remove samples at the indicated steps to monitor the procedure on an analytical gel (see page 55).
- The ▲ symbol denotes values for QIAGEN-tip 2500, using the QIAGEN Plasmid Mega Kit; ● denotes values for QIAGEN-tip 10000, using the QIAGEN Plasmid Giga Kit.

## Things to do before starting

- Before use, centrifuge RNase A briefly, and then add into Buffer P1 to obtain a final concentration of 100 µg/mL.
- Check Buffer P2 for SDS precipitation due to low storage temperatures. If necessary, dissolve the SDS by warming to 37°C.
- Prechill Buffer P3 at 4°C.
- **Optional:** Add the provided LyseBlue reagent to Buffer P1 and mix before use. Use 1 vial LyseBlue reagent per bottle Buffer P1 for a final dilution of 1:1000 (e.g., 10 µL LyseBlue into 10 mL Buffer P1). LyseBlue provides visual identification of optimum buffer mixing thereby preventing the common handling errors that lead to inefficient cell lysis and incomplete precipitation of SDS, genomic DNA, and cell debris. For more details, see “Using LyseBlue reagent” on page 16.
- **Optional:** If using a QIAfilter Mega-Giga Cartridges (cat. no. 19781) for lysate clearing, screw the QIAfilter Mega-Giga Cartridge onto a 45 mm-neck glass bottle and connect it to a vacuum source. Do not overtighten the QIAfilter Cartridge on the bottle neck, because the QIAfilter Cartridge plastic may crack.

## Procedure

1. Pick a single colony from a freshly streaked selective plate, and inoculate a starter culture of 5–10 mL LB medium containing the appropriate selective antibiotic. Incubate for approximately 8 h at 37°C with vigorous shaking (approx. 300 rpm).

Use a tube or flask with a volume at least 4 times the volume of the culture.

2. Dilute the starter culture 1/500 to 1/1000 into selective LB medium.

For high-copy plasmids, inoculate ▲ 500 mL or ● 2.5 L medium with ▲ 500–1000 µL or ● 2.5–5 mL of starter culture.

For low-copy plasmids, inoculate ▲ 2.5 L or ● 5 L medium with ▲ 2.5–5 mL or ● 5–10 mL of starter culture.

Grow at 37°C for 12–16 h with vigorous shaking (approx. 300 rpm).

Use a flask or vessel with a volume at least 4 times the volume of the culture. The culture should reach a cell density of approximately  $3\text{--}4 \times 10^9$  cells per milliliter, which typically corresponds to a pellet wet weight of approximately 3 g/L medium.

3. Harvest the bacterial cells by centrifugation at  $6000 \times g$  for 15 min at 4°C.

**Note:** For Giga preparations of low-copy plasmids using 5 L of culture, volumes of Buffers P1, P2, and P3 in steps 4–6 should be doubled, due to the very large number of cells harvested. For routine Giga preparation of low-copy plasmids, additional Buffers P1, P2, and P3 may need to be purchased (see “Ordering Information”, page 60) or prepared (see “Preparation of buffers”, page 59).

If you wish to stop the protocol and continue later, freeze the cell pellets at –30 to –15°C.

4. Resuspend the bacterial pellet in ▲ 50 mL or ● 125 mL of Buffer P1.

For efficient lysis, it is important to use a vessel that is large enough to allow complete mixing of the lysis buffers. We recommend a 500 mL bottle for Mega preparations and a 1000 mL bottle for Giga preparations. Ensure that RNase A has been added to Buffer P1.

If LyseBlue reagent has been added to Buffer P1, vigorously shake the buffer bottle before use to ensure LyseBlue particles are completely resuspended. The bacteria should be resuspended completely by vortexing or pipetting up and down until no cell clumps remain.

5. Add ▲ 50 mL or ● 125 mL of Buffer P2, mix thoroughly by vigorously inverting 4–6 times, and incubate at room temperature for 5 min.

Do not vortex, because this will result in shearing of genomic DNA. The lysate should appear viscous. Do not allow the lysis reaction to proceed for more than 5 min. After use, the bottle containing Buffer P2 should be closed immediately to avoid acidification of Buffer P2 from CO<sub>2</sub> in the air.

If LyseBlue has been added to Buffer P1, the cell suspension will turn blue after addition of Buffer P2. Mixing should result in a homogeneously colored suspension. If the suspension contains localized colorless regions or if brownish cell clumps are still visible, continue mixing the solution until a homogeneously colored suspension is achieved.

6. Add ▲ 50 mL or ● 125 mL of chilled Buffer P3, mix immediately and thoroughly by vigorously inverting 4–6 times, and incubate on ice for 30 min.

Precipitation is enhanced by using chilled Buffer P3 and incubating on ice. After addition of Buffer P3, a fluffy white material forms and the lysate becomes less viscous. The precipitated material contains genomic DNA, proteins, cell debris, and KDS. The lysate should be mixed thoroughly to avoid localized potassium dodecyl sulfate precipitation.

If LyseBlue reagent has been used, the suspension should be mixed until all trace of blue has gone and the suspension is colorless. A homogeneous colorless suspension indicates that the SDS has been effectively precipitated.

**Optional:** If using a QIAfilter for lysate clearing instead of centrifugation go to step 9.

7. Centrifuge at  $\geq 20,000 \times g$  for 30 min at 4°C. Remove supernatant containing plasmid DNA promptly.

Before loading the centrifuge, the sample should be mixed again. Centrifugation should be performed in 250 or 500 mL non-glass tubes (e.g., polypropylene; not supplied).

**Note:** Instead of centrifugation steps 7 and 8, the lysate can be efficiently cleared by filtration using a QIAfilter Kits or Cartridges (see [www.qiagen.com/products/discovery-and-translational-research/dna-rna-purification/dna-purification/plasmid-dna/qiafilter-plasmid-kits](http://www.qiagen.com/products/discovery-and-translational-research/dna-rna-purification/dna-purification/plasmid-dna/qiafilter-plasmid-kits)).

8. Centrifuge the supernatant again at  $\geq 20,000 \times g$  for 15 min at 4°C. Remove supernatant containing plasmid DNA promptly.

This step should be carried out to avoid applying suspended or particulate material to the QIAGEN-tip. Suspended material (causing the sample to appear turbid) can clog the QIAGEN-tip and reduce or eliminate gravity flow.

**Optional:** Remove a ▲ 120  $\mu\text{L}$  or ● 75  $\mu\text{L}$  sample from the cleared lysate supernatant and save for an analytical gel (sample 1) to determine whether growth and lysis conditions were optimal.

**Note:** After this step, proceed to step 12. Steps 9–11 should be skipped if not using the QIAfilter for clearing of the lysate.

9. Pour the lysate into the QIAfilter Mega-Giga Cartridge and incubate at room temperature for 10 min.

**Important:** This 10 min incubation at room temperature is essential for optimal performance of the QIAfilter Mega-Giga Cartridge. Do not agitate the QIAfilter Cartridge during this time. A precipitate containing proteins, genomic DNA, and detergent will float and form a layer on top of the solution. This ensures convenient filtration without clogging.

10. Switch on the vacuum source. After all liquid has been pulled through, switch off the vacuum source. Leave the QIAfilter Cartridge attached.
11. Add 50 mL (both ▲ Mega and ● Giga) Buffer FWB2 to the QIAfilter Cartridge and gently stir the precipitate using a sterile spatula. Switch on the vacuum source until the liquid has been pulled through completely. Gentle stirring of the precipitate enhances the flow of liquid through the filter unit. Take care not to disperse the precipitate, as this may result in carryover of cell debris and KDS, which will affect flow and binding characteristics of the QIAGEN column. The filtered lysate in the bottle contains the plasmid DNA.

**Optional:** Remove a ▲ 120  $\mu$ L or ● 75  $\mu$ L sample from the cleared lysate and save for an analytical gel (sample 1) to determine whether growth and lysis conditions were optimal.

12. Equilibrate a ▲ QIAGEN-tip 2500 or ● QIAGEN-tip 10000 by applying ▲ 35 mL or ● 75 mL Buffer QBT, and allow the column to empty by gravity flow.

Flow of buffer will begin automatically by reduction in surface tension due to the presence of detergent in the equilibration buffer. Allow the QIAGEN-tip to drain completely. QIAGEN-tips can be left unattended because the flow of buffer will stop when the meniscus reaches the upper frit in the column.

13. Apply the supernatant from step 8 to the QIAGEN-tip and allow it to enter the resin by gravity flow.

The supernatant should be loaded onto the QIAGEN-tip promptly. If it is left too long and becomes cloudy due to further precipitation of protein, it must be centrifuged again or filtered before loading to prevent clogging of the QIAGEN-tip.

**Optional:** Remove a ▲ 120  $\mu$ L or ● 75  $\mu$ L sample from the flow-through and save for an analytical gel (sample 2) to determine efficiency of DNA binding to the QIAGEN resin.

14. Wash the QIAGEN-tip with a total of ▲ 200 mL or a total of ● 600 mL Buffer QC.

Allow Buffer QC to move through the QIAGEN-tip by gravity flow. The first half of the volume of wash buffer is sufficient to remove contaminants in the majority of plasmid DNA preparations. The second half is particularly necessary when large culture volumes or bacterial strains producing large amounts of carbohydrates are used.

**Optional:** Remove a ▲ 160  $\mu$ L or ● 120  $\mu$ L sample from the combined wash fractions and save for an analytical gel (sample 3).

15. Elute DNA with ▲ 35 mL or ● 100 mL Buffer QF.

Use of polycarbonate centrifuge tubes for collection is not recommended because polycarbonate is not resistant to the alcohol used in subsequent steps.

**Optional:** Remove a ▲ 22  $\mu$ L or ● 20  $\mu$ L sample of the eluate and save for an analytical gel (sample 4).

**Note:** For constructs larger than 45–50 kb, prewarming the elution buffer to 65°C may help to increase yield.

If you wish to stop the protocol and continue later, store the eluate at 4°C. Storage periods longer than overnight are not recommended.

16. Precipitate DNA by adding ▲ 24.5 mL or ● 70 mL (0.7 volumes) room-temperature isopropanol to the eluted DNA. Mix and centrifuge immediately at  $\geq 15,000 \times g$  for 30 min at 4°C. Carefully decant the supernatant.

All solutions should be at room temperature to minimize salt precipitation, although centrifugation is carried out at 4°C to prevent overheating of the sample. Alternatively, disposable conical-bottom centrifuge tubes can be used for centrifugation at  $5000 \times g$  for 60 min at 4°C. Isopropanol pellets have a glassy appearance and may be more difficult to see than the fluffy, salt-containing pellets that result from ethanol precipitation. Marking the outside of the tube before centrifugation allows the pellet to be more easily located. Isopropanol pellets are also more loosely attached to the side of the tube, and care should be taken when removing the supernatant.

17. Wash DNA pellet with ▲ 7 mL or ● 10 mL of room-temperature 70% ethanol, and centrifuge at  $\geq 15,000 \times g$  for 10 min. Carefully decant the supernatant without disturbing the pellet.

Alternatively, disposable conical-bottom centrifuge tubes (not supplied) can be used for centrifugation at  $5000 \times g$  for 60 min at 4°C. The 70% ethanol removes precipitated salt and replaces isopropanol with the more volatile ethanol, making the DNA easier to redissolve.

18. Air-dry the pellet for 10–20 min, and redissolve the DNA in a suitable volume of buffer (e.g., TE buffer, pH 8.0, or 10 mM Tris·Cl, pH 8.5).

Redissolve the DNA pellet by rinsing the walls to recover the DNA, especially if glass tubes have been used. Pipetting the DNA up and down to promote resuspension may cause shearing and should be avoided. Overdrying the pellet will make the DNA difficult to redissolve. DNA dissolves best under slightly alkaline conditions; it does not easily dissolve in acidic buffers.

## Determination of yield

To determine the yield, DNA concentration should be determined by both UV spectrophotometry at 260 nm and quantitative analysis on an agarose gel. For reliable spectrophotometric DNA quantification,  $A_{260}$  readings should lie between 0.1 and 1.0.

## Agarose gel analysis

We recommend removing and saving aliquots during the purification procedure (samples 1–4). If the plasmid DNA is of low yield or quality, the samples can be analyzed by agarose gel electrophoresis to determine the stage of the purification procedure where the problem occurred (see page 55).

# Protocol: Very Low-Copy Plasmid/Cosmid Purification Using QIAGEN-tip 100 or QIAGEN-tip 500

Very low-copy plasmids and cosmids of less than 10 copies per cell often require large culture volumes to yield significant amounts of DNA (for additional information, see [www.qiagen.com/goto/plasmidinfo](http://www.qiagen.com/goto/plasmidinfo)). This protocol is suitable for QIAGEN-tip 100 or QIAGEN-tip 500. After alkaline lysis, there is an additional isopropanol precipitation step to decrease the amount of lysate before DNA is bound to the QIAGEN-tip. Culture volumes and tip sizes are selected to match the quantity of DNA expected to the capacity of the QIAGEN-tip. For purification of P1 and BAC DNA using QIAGEN-tips, please contact QIAGEN Technical Services at [support.qiagen.com](mailto:support.qiagen.com). For purification of large cosmid and plasmid DNA constructs, for example, BAC, PAC, or P1 DNA, the QIAGEN Large-Construct Kit is available (see "Ordering Information", page 61).

Details of yields, culture volumes, QIAGEN-tip sizes, and buffer volumes to be used for purification of very low-copy plasmids and cosmids are given in Table 5.

**Table 5. Parameters for purification of very low-copy plasmids and cosmids of less than 10 copies per cell**

Required DNA yield*	Up to 100 µg	Up to 500 µg
Culture volume	500 mL	2.5 L
Buffer P1†	20 mL	125 mL
Buffer P2†	20 mL	125 mL
Buffer P3†	20 mL	125 mL
<b>QIAGEN-tip</b>	<b>QIAGEN-tip 100</b>	<b>QIAGEN-tip 500</b>
Buffer QBT (for equilibration)	4 mL	10 mL
Buffer QC (for washing)	2 x 10 mL	2 x 30 mL
Buffer QF (for elution)	5 mL	15 mL

\* For very-low-copy plasmids, expected yields are 20–100 µg for the QIAGEN-tip 100 and 100–500 µg for the QIAGEN-tip 500.

† Volumes of lysis Buffers P1, P2, and P3 are higher than in the standard protocols on pages 24–31 to efficiently lyse the large number of cells required for purification of very low-copy plasmids and cosmids.

## Important points before starting

- New users are advised to familiarize themselves with the detailed protocol provided in this handbook. In addition, extensive background information is provided on our plasmid resource page, [www.qiagen.com/goto/plasmidinfo](http://www.qiagen.com/goto/plasmidinfo).
- If working with low-copy vectors, it may be beneficial to increase the lysis buffer volumes to increase the efficiency of alkaline lysis, and thereby the DNA yield. In case additional Buffers P1, P2, and P3 are needed, their compositions are provided in Appendix B, page 55. Alternatively, the buffers may be purchased separately (see “Ordering Information”, page 61).
- **Optional:** Remove samples at the indicated steps to monitor the procedure on an analytical gel (see page 55).
- The ▲ symbol denotes values for QIAGEN-tip 100, using the QIAGEN Plasmid Midi Kit; ● denotes values for QIAGEN-tip 500, using the QIAGEN Plasmid Maxi Kit.

## Things to do before starting

- Before use, centrifuge RNase A briefly, and then add into Buffer P1 to obtain a final concentration of 100 µg/mL.
- Check Buffer P2 for SDS precipitation due to low storage temperatures. If necessary, dissolve the SDS by warming to 37°C.
- Prechill Buffer P3 at 4°C.
- **Optional:** Add the provided LyseBlue reagent to Buffer P1 and mix before use. Use 1 vial LyseBlue reagent per bottle Buffer P1 for a final dilution of 1:1000 (e.g., 10 µL LyseBlue into 10 mL Buffer P1). LyseBlue provides visual identification of optimum buffer mixing thereby preventing the common handling errors that lead to inefficient cell lysis and incomplete precipitation of SDS, genomic DNA, and cell debris. For more details, see "Using LyseBlue reagent" on page 16.

## Procedure

1. Pick a single colony from a freshly streaked selective plate, and inoculate a starter culture of 2–10 mL LB medium containing the appropriate selective antibiotic. Incubate for approximately 8 h at 37°C with vigorous shaking (approx. 300 rpm).

Use a tube or flask with a volume of at least 4 times the volume of the culture.

2. Dilute the starter culture 1/500 to 1/1000 into ▲ 500 mL or ● 2.5 L of selective LB medium using ▲ 500–1000 µL or ● 2.5–5 mL of starter culture. Grow at 37°C for 12–16 h with vigorous shaking (approx. 300 rpm).

Use a flask or vessel with a volume of at least 4 times the volume of the culture. The culture should reach a cell density of approximately  $3\text{--}4 \times 10^9$  cells per mL, which typically corresponds to a pellet wet weight of approximately 3 g/L medium.

3. Harvest the bacterial cells by centrifugation at  $6000 \times g$  for 15 min at 4°C.

If you wish to stop the protocol and continue later, freeze the cell pellets at  $-30$  to  $-15^{\circ}\text{C}$ .

4. Resuspend the bacterial pellet in ▲ 20 mL or ● 125 mL Buffer P1.

For efficient lysis, it is important to use a vessel that is large enough to allow complete mixing of the lysis buffers. Ensure that RNase A has been added to Buffer P1.

If LyseBlue reagent has been added to Buffer P1, vigorously shake the buffer bottle before use to ensure LyseBlue particles are completely resuspended. The bacteria should be resuspended completely by vortexing or pipetting up and down until no cell clumps remain.

5. Add ▲ 20 mL or ● 125 mL Buffer P2, mix thoroughly by vigorously inverting the sealed tube 4–6 times, and incubate at room temperature for 5 min.

Do not vortex, because this will result in shearing of genomic DNA. The lysate should appear viscous. Do not allow the lysis reaction to proceed for more than 5 min. After use, the bottle containing Buffer P2 should be closed immediately to avoid acidification of Buffer P2 from  $\text{CO}_2$  in the air.

If LyseBlue has been added to Buffer P1, the cell suspension will turn blue after addition of Buffer P2. Mixing should result in a homogeneously colored suspension. If the suspension contains localized colorless regions or if brownish cell clumps are still visible, continue mixing the solution until a homogeneously colored suspension is achieved.

6. Add ▲ 20 mL or ● 125 mL chilled Buffer P3, mix immediately and thoroughly by vigorously inverting 4–6 times, and incubate on ice for 30 min.

Precipitation is enhanced by using chilled Buffer P3 and incubating on ice. After addition of Buffer P3, a fluffy white material forms and the lysate becomes less viscous. The precipitated material contains genomic DNA, proteins, cell debris, and KDS. The lysate should be mixed thoroughly to avoid localized potassium dodecyl sulfate precipitation.

If LyseBlue reagent has been used, the suspension should be mixed until all trace of blue has gone and the suspension is colorless. A homogeneous colorless suspension indicates that the SDS has been effectively precipitated.

7. Centrifuge at  $\geq 20,000 \times g$  for 30 min at 4°C. Remove supernatant containing plasmid DNA promptly.

Before loading the centrifuge, the sample should be mixed again. Centrifugation should be performed in non-glass tubes (e.g., polypropylene; not supplied). After centrifugation, the supernatant should be clear.

8. Centrifuge the supernatant again at  $\geq 20,000 \times g$  for 15 min at 4°C. Remove supernatant containing plasmid DNA promptly. Alternatively, the sample can be filtered over a prewetted, folded filter.

This second centrifugation step completely clears the lysate of precipitated material.

**Optional:** Remove a ▲ 600  $\mu\text{L}$  or ● 750  $\mu\text{L}$  sample from the cleared lysate supernatant and save for an analytical gel (sample 1) to determine whether growth and lysis conditions were optimal.

9. Precipitate the DNA by adding ▲ 42 mL or ● 262.5 mL (0.7 volumes) of room-temperature isopropanol to the lysate. Centrifuge at  $\geq 15,000 \times g$  for 30 min at 4°C, and carefully decant the supernatant.

This isopropanol precipitation reduces the sample volume to facilitate loading of the column. It also serves to remove unwanted metabolites such as proteins and lipopolysaccharides.

10. Redissolve the DNA pellet in 500  $\mu\text{L}$  TE buffer, pH 8.0, and add Buffer QBT to obtain a final volume of ▲ 5 mL or ● 12 mL for selected ▲ QIAGEN-tip 100 or ● QIAGEN-tip 500, respectively.

TE buffer is used to facilitate redissolving of the DNA. Buffer QBT provides optimal DNA binding conditions.

11. Equilibrate a ▲ QIAGEN-tip 100 or ● QIAGEN-tip 500 by applying ▲ 4 mL or ● 10 mL Buffer QBT, and allow the column to empty by gravity flow.

Flow of buffer will begin automatically by reduction in surface tension due to the presence of detergent in the equilibration buffer. Allow the QIAGEN-tip to drain completely. QIAGEN-tips can be left unattended because the flow of buffer will stop when the meniscus reaches the upper frit in the column.

12. Apply the DNA solution from step 10 to the QIAGEN-tip and allow it to enter the resin by gravity flow.

**Optional:** Remove a ▲ 50  $\mu$ L or ● 24  $\mu$ L sample from the flow-through and save for an analytical gel (sample 2) to determine the efficiency of DNA binding to the QIAGEN resin.

13. Wash the QIAGEN-tip with ▲ 2 x 10 mL or ● 2 x 30 mL Buffer QC.

Allow Buffer QC to move through the QIAGEN-tip by gravity flow. The first wash is sufficient to remove contaminants in the majority of plasmid DNA preparations. The second wash is particularly necessary when large culture volumes or bacterial strains producing large amounts of carbohydrates are used.

**Optional:** Remove a ▲ 200  $\mu$ L or ● 120  $\mu$ L sample from the combined wash fractions and save for an analytical gel (sample 3).

14. Elute DNA with ▲ 5 mL or ● 15 mL Buffer QF.

Use of polycarbonate tubes (not supplied) to collect the eluate is not recommended as polycarbonate is not resistant to the alcohol used in subsequent steps.

**Note:** For constructs larger than 45–50 kb, prewarming the elution buffer to 65°C may help to increase yield.

**Optional:** Remove a ▲ 50  $\mu$ L or ● 30  $\mu$ L sample of the eluate and save for an analytical gel (sample 4).

If you wish to stop the protocol and continue later, store the eluate at 4°C. Storage periods longer than overnight are not recommended.

15. Precipitate DNA by adding ▲ 3.5 mL or ● 10.5 mL (0.7 volumes) of room-temperature isopropanol to the eluted DNA. Mix and centrifuge immediately at  $\geq 15,000 \times g$  for 30 min at 4°C. Carefully decant the supernatant.

All solutions should be at room temperature to minimize salt precipitation, although centrifugation is carried out at 4°C to prevent overheating of the sample. Alternatively, disposable conical-bottom centrifuge tubes (not supplied) can be used for centrifugation at  $5000 \times g$  for 60 min at 4°C. Isopropanol pellets have a glassy appearance and may be more difficult to see than the fluffy, salt-containing pellets that result from ethanol precipitation. Marking the outside of the tube before centrifugation allows the pellet to be more easily located. Isopropanol pellets are also more loosely attached to the side of the tube, and care should be taken when removing the supernatant.

16. Wash DNA pellet with ▲ 2 mL or ● 5 mL room-temperature 70% ethanol, and centrifuge at  $\geq 15,000 \times g$  for 10 min. Carefully decant the supernatant without disturbing the pellet.

Alternatively, disposable conical-bottom centrifuge tubes (not supplied) can be used for centrifugation at  $5000 \times g$  for 60 min at 4°C. The 70% ethanol removes precipitated salt and replaces isopropanol with the more volatile ethanol, making the DNA easier to redissolve.

17. Air-dry the pellet for 5–10 min, and redissolve the DNA in a suitable volume of buffer (e.g., TE buffer, pH 8.0, or 10 mM Tris-Cl, pH 8.5).

Redissolve DNA pellet by rinsing the walls to recover the DNA, especially if glass tubes have been used. Pipetting the DNA up and down to promote resuspension may cause shearing and should be avoided. Overdrying the pellet will make the DNA difficult to redissolve. DNA dissolves best under alkaline conditions; it does not easily dissolve in acidic buffers.

## Determination of yield

To determine the yield, DNA concentration should be determined by both UV spectrophotometry and quantitative analysis on an agarose gel.

## Agarose gel analysis

We recommend removing and saving aliquots during the purification procedure (samples 1–4). If the plasmid DNA is of low yield or quality, the samples can be analyzed by agarose gel electrophoresis to determine the stage of the purification procedure where the problem occurred (see page 55).

# Troubleshooting Guide

This troubleshooting guide may be helpful in solving any problems that may arise. For more information, see also the Frequently Asked Questions page in our Technical Support Center: [www.qiagen.com/FAQ/FAQList.aspx](http://www.qiagen.com/FAQ/FAQList.aspx). The scientists in QIAGEN Technical Services are always happy to answer any questions you may have about either the information or protocols in this handbook (for contact information, visit [support.qiagen.com](http://support.qiagen.com)).

## Comments and suggestions

---

### Low or no DNA yield

#### No DNA in lysate (sample 1)

- |   |   |
|---|---|
| a) Plasmid did not propagate                | Please read "Growth of Bacterial Cultures" on our web page <a href="http://www.qiagen.com/goto/plasmidinfo">www.qiagen.com/goto/plasmidinfo</a> , and check that the conditions for optimal growth were met.  |
| b) Alkaline lysis was inefficient           | <p>If cells have grown to very high densities or a larger amount of cultured medium than recommended was used, the ratio of biomass to lysis reagent is shifted. This may result in poor lysis conditions, because the volumes of Buffers P1, P2, and P3 are not sufficient for setting the plasmid DNA free efficiently. Reduce culture volume or increase volumes of Buffers P1, P2, and P3.</p> <p>Also, insufficient mixing of lysis reagents will result in reduced yield. Mix thoroughly after addition of Buffers P1, P2, and P3 to achieve homogeneous suspensions. Use LyseBlue to visualize efficiency of mixing.</p> |
| c) Insufficient lysis for low-copy plasmids | For low copy-plasmid preparations, doubling the volumes of lysis Buffers P1, P2, and P3 may help to increase plasmid yield and quality (see page 40 and background on our web page <a href="http://www.qiagen.com/goto/plasmidinfo">www.qiagen.com/goto/plasmidinfo</a> ).  |
| d) Lysate incorrectly prepared              | <p>Check Buffer P2 for SDS precipitation resulting from low storage temperatures and dissolve the SDS by warming. The bottle containing Buffer P2 should always be closed immediately after use. Lysis buffers prepared in the laboratory should be prepared according to the instructions on page 59.</p> <p>If necessary, prepare fresh Buffers P1, P2, and P3.</p>   |

## Comments and suggestions

---

### DNA in flow-through fraction (sample 2)

- |    |  |  |
|----|--|--|
| a) | Column was overloaded                          | Check the culture volume and yield against the capacity of the QIAGEN-tip, as detailed at the beginning of each protocol. Reduce the culture volume accordingly, or select a larger QIAGEN-tip if a higher yield is desired. For very low-copy number plasmid and cosmid preps requiring very large culture volumes, please see page 40. |
| b) | SDS (or other ionic detergent) was in lysate   | Chill Buffer P3 before use. If the lysate is cleared by centrifugation, load onto QIAGEN-tip promptly after centrifugation. If lysate is too viscous for effective mixing of Buffer P3, reduce culture volume or increase volumes of Buffers P1, P2, and P3.<br>Use LyseBlue to visualize efficiency of mixing.                          |
| c) | Inappropriate salt or pH conditions in buffers | Ensure that any buffers prepared in the laboratory were prepared according to the instructions provided on page 59.  |
| d) | Column flow was uneven                         | Store QIAGEN-tips at room temperature. If stored under cold, damp conditions for prolonged periods of time, the resin may clump. This problem can be overcome by shaking the column before use.  |

### DNA in Buffer QC wash fraction (sample 3)

- |    |                         |  |
|----|-------------------------|--|
| a) | Column was overloaded   | Check the culture volume and yield against the capacity of the QIAGEN-tip, as detailed at the beginning of each protocol. Reduce the culture volume accordingly, or select a larger QIAGEN-tip if a higher yield is desired. For very low-copy-number plasmid and cosmid preps requiring very large culture volumes, please see page 40. |
| b) | Buffer QC was incorrect | Check pH and salt concentration of Buffer QC. Recover DNA by precipitation, and purify on a new QIAGEN-tip. For details, please refer to <a href="http://www.qiagen.com/goto/plasmidinfo">www.qiagen.com/goto/plasmidinfo</a> .  |

### No DNA in eluate (sample 4)

- |    |   |   |
|----|---|---|
| a) | No DNA in the lysate                                    | See section "No DNA in lysate (sample 1)", page 48.   |
| b) | Elution Buffer QF or QN was incorrect                   | Check pH and salt concentration of Buffer QF or QN. Recover DNA by eluting with fresh buffer. |
| c) | DNA passed through in the flow-through or wash fraction | See previous two sections.  |

## Comments and suggestions

---

### Little or no DNA after precipitation

- |    |                            |  |
|----|----------------------------|--|
| a) | DNA failed to precipitate  | Ensure that the precipitate is centrifuged at $\geq 15,000 \times g$ for 30 min. Recover DNA by centrifuging for longer and at higher speeds. Try another isopropanol batch.   |
| b) | DNA pellet was lost        | Isopropanol pellets are glassy and may be difficult to see. Mark the outside of the tube before centrifugation. Isopropanol pellets may also be loosely attached to the side of the tube, so pour supernatant off gently.  |
| c) | DNA was poorly redissolved | Check that DNA is completely redissolved. Be sure to wash any DNA off the walls, particularly if glass tubes and a fixed-angle rotor are used. Up to half of the total DNA may be smeared on the walls. Alternatively, a swinging bucket rotor can be used to ensure that the pellet is located at the bottom of the tube. |

### Plasmid DNA difficult to redissolve

- |    |                                |   |
|----|--------------------------------|---|
| a) | Pellet was overdried           | Air-dry pellet instead of using a vacuum, especially if the DNA is of high molecular weight. Redissolve DNA by warming the solution slightly and allowing more time for redissolving.   |
| b) | Residual isopropanol in pellet | Ensure that pellets are washed with 70% ethanol to remove traces of isopropanol. Redissolve DNA by warming the solution slightly and allowing more time for redissolving. Increase volume of buffer used for redissolving if necessary. |
| c) | Too much salt in pellet        | Ensure that isopropanol is at room temperature for precipitation, and wash the pellet twice with room temperature 70% ethanol. Recover DNA by increasing the volume of buffer used for redissolving.                                    |
| d) | Buffer pH was too low          | Ensure that the pH of the buffer used for redissolving is $\geq 8.0$ because DNA does not dissolve well in acidic solutions.  |
| e) | Resuspension volume too low    | Increase resuspension volume if the solution above the pellet is highly viscous.  |

### Contaminated DNA/poor-quality DNA

- |    |                           |  |
|----|---------------------------|--|
| a) | Genomic DNA in the eluate | Mixing of bacterial lysate was too vigorous. The lysate must be handled gently after addition of Buffers P2 and P3 to prevent shearing of chromosomal DNA. Reduce culture volume if lysate is too viscous for gentle mixing. |
|----|---------------------------|--|

## Comments and suggestions

---

- |   |   |
|---|---|
| b) RNA in the eluate                      | RNase A digestion was insufficient. Check culture volume against recommended volumes, and reduce if necessary. Check that the RNase A provided with the kit has been used. If Buffer P1 is more than 6 months old, add more RNase A. Recover DNA by precipitating the eluate, digesting with RNase A, and purifying on a new QIAGEN-tip as detailed in <a href="http://www.qiagen.com/goto/plasmidinfo">www.qiagen.com/goto/plasmidinfo</a> . |
| c) Nuclease contamination                 | Check buffers for nuclease contamination and replace if necessary. Use new glass- and plasticware, and wear gloves.   |
| d) Lysis time was too long                | Ensure that lysis step (Buffer P2) does not exceed 5 min.   |
| e) Overloaded alkaline lysis              | Check the culture volume and yield against the capacity of the QIAGEN-tip. Reduce the culture volume accordingly or alternatively increase the volumes of Buffers P1, P2, and P3.   |
| f) Plasmid DNA is nicked/sheared/degraded | DNA was poorly buffered. Redissolve DNA in TE buffer, pH 8.0, to inhibit nuclease activity and maintain stable pH during storage.   |
| g) Endonuclease-containing host           | Refer to background information on <a href="http://www.qiagen.com/goto/plasmidinfo">www.qiagen.com/goto/plasmidinfo</a> and consider changing <i>Escherichia coli</i> host strain.  |
| h) Shearing during redissolving           | Redissolve DNA gently, without vortexing or vigorous pipetting. Avoid using small pipette tips.   |
| i) Particles in redissolved DNA           | Centrifuge the DNA solution and transfer supernatant to a new tube. The particles have no effect on DNA quality. Alternatively, use HiSpeed kits containing QIAprecipitator, which filters the eluate.  |

## Poor DNA performance

- |                            |  |
|----------------------------|--|
| a) Too much salt in pellet | Ensure that isopropanol is at room temperature for precipitation, and wash the pellet twice with room temperature 70% ethanol. Precipitate the DNA again to remove the salt.   |
| b) Residual protein        | Check culture volume against the recommended volumes and reduce if necessary. Ensure that the bacterial lysate is cleared properly by centrifugation at $\geq 20,000 \times g$ for 45 min, or using a QIAfilter Cartridge. |

## Comments and suggestions

---

### Extra DNA bands on analytical gel

- |    |   |  |
|----|---|--|
| a) | Dimer form of plasmid                   | Dimers or multimers of supercoiled plasmid DNA are formed during replication of plasmid DNA. Typically, when purified plasmid DNA is electrophoresed, both the supercoiled monomer and dimer form of the plasmid are detected upon ethidium bromide staining of the gel (see Figure 4, page 55). The ratio of these forms is often host dependent. |
| b) | Plasmid has formed denatured supercoils | This species runs faster than closed circular DNA on a gel and is resistant to restriction digestion (see Figure 4, page 55). Do not incubate cells for longer than 5 min in Buffer P2. Mix immediately after addition of Buffer P3.   |
| c) | Possible deletion mutants               | Some sequences are poorly maintained in plasmids. Check for deletions by restriction analysis. Cosmid clones, in particular, should always be prepared from freshly streaked, well-isolated colonies because cosmids are not stable in <i>E. coli</i> for long periods of time.  |

### Blocked QIAGEN-tip

- |                   |  |
|-------------------|--|
| Lysate was turbid | Ensure that the lysate is clear before it is loaded onto the column. Ensure that Buffer P3 is chilled before use. Check <i>g</i> -force and centrifugation time. Alternatively, clear the lysate using a QIAfilter Cartridge. To clear a blocked QIAGEN-tip, positive pressure may be applied (e.g., by using a syringe fitted into a rubber stopper with a hole). |
|-------------------|--|

### QIAfilter Cartridge clogs during filtration

- |    |  |  |
|----|--|--|
| a) | Too large culture volume used  | Use no more than the culture volume recommended in the protocol.   |
| b) | Inefficient mixing after addition of Buffer P3                             | Mix well until a fluffy white material has formed and the lysate is no longer viscous.   |
| c) | Mixing too vigorous after addition of Buffer P3                            | After addition of Buffer P3 the lysate should be mixed immediately but gently. Vigorous mixing disrupts the precipitate into tiny particles which may clog the QIAfilter Cartridge.  |
| d) | QIAfilter Cartridge was not loaded immediately after addition of Buffer P3 | After addition of Buffer P3 the lysate should be loaded immediately after being poured into the QIAfilter Cartridge. Decanting after incubation may disrupt the precipitate into tiny particles which may clog the QIAfilter Cartridge.    |
| e) | QIAfilter Cartridge was not agitated during incubation                     | Pour the lysate into the QIAfilter Cartridge immediately after addition of Buffer P3 and do not agitate during the 10 minute incubation. Agitation causes the precipitate to be disrupted into tiny particles, instead of forming a layer. |

### Comments and suggestions

---

- |    |   |   |
|----|---|---|
| f) | Incubation after addition of Buffer P3 on ice instead of at RT      | Ensure incubation is performed at room temperature in the QIAfilter Cartridge. Precipitate flotation is more efficient at room temperature than on ice.   |
| g) | Incubation time after addition of Buffer P3 too short               | Incubate with Buffer P3 as indicated in the protocol. If the precipitate has not risen to the top after the 10 minute incubation, carefully run a sterile pipet tip or sterile spatula around the cartridge wall to dislodge the precipitate before continuing with the filtration. |
| h) | Vacuum was weak or negligible (QIAfilter Mega-Giga Cartridges only) | Ensure that the vacuum generates a vacuum pressure of –200 to –600 millibars (–150 to –450 mg Hg).  |

#### **QIAfilter Cartridge clogs after addition of Buffer FWB2**

(QIAfilter Mega-Giga Cartridges only)

Precipitate was not stirred after addition of Buffer FWB2	After addition of Buffer FWB2 to the QIAfilter Mega-Giga Cartridge, gently stir the precipitate using a sterile spatula.
---	--

#### **Lysate not clear after filtration**

(QIAfilter Midi and Maxi Cartridges only)

Precipitate was forced through the QIAfilter Cartridge	Filter until all of the lysate has passed through the QIAfilter Midi or Maxi Cartridge, but do not apply extreme force. Approximately 10 mL (QIAfilter Midi) or 25 mL (QIAfilter Maxi) of lysate are typically recovered.
--	---

# Appendix A: Agarose Gel Analysis of the Purification Procedure

DNA yields and quality can be readily analyzed by agarose gel electrophoresis. Poor yields and quality can be caused by a number of different factors. To determine the stage of the procedure where the problem occurred, save fractions from different steps of the purification procedure (see below and Table 6) and analyze by agarose gel electrophoresis.

## Preparation of samples

Remove aliquots from the cleared lysate (sample 1), flow-through (sample 2), combined Buffer QC wash fractions (sample 3), and Buffer QF/QN eluate (sample 4), as indicated in each protocol and in Table 6. Precipitate the nucleic acids with 1 volume of isopropanol, rinse the pellets with 70% ethanol, drain well, and resuspend in 10  $\mu$ L TE buffer, pH 8.0.

**Table 6. Sample volumes required for agarose gel analysis**

Sample	Protocol step	Very low-copy plasmids/cosmids						
		QIAGEN-tip						
		Mini	Midi	Maxi	Mega	Giga	100	500
1	Cleared lysate	50 $\mu$ L	240 $\mu$ L	120 $\mu$ L	120 $\mu$ L	75 $\mu$ L	600 $\mu$ L	750 $\mu$ L
2	Flow-through	50 $\mu$ L	240 $\mu$ L	120 $\mu$ L	120 $\mu$ L	75 $\mu$ L	50 $\mu$ L	24 $\mu$ L
3	Combined wash fractions	220 $\mu$ L	400 $\mu$ L	240 $\mu$ L	160 $\mu$ L	120 $\mu$ L	200 $\mu$ L	120 $\mu$ L
4	Eluate	45 $\mu$ L	100 $\mu$ L	60 $\mu$ L	22 $\mu$ L	20 $\mu$ L	50 $\mu$ L	30 $\mu$ L
<b>% of prep represented by each sample volume</b>		5.50%	2.00%	0.40%	0.08%	0.02%	1.00%	0.20%

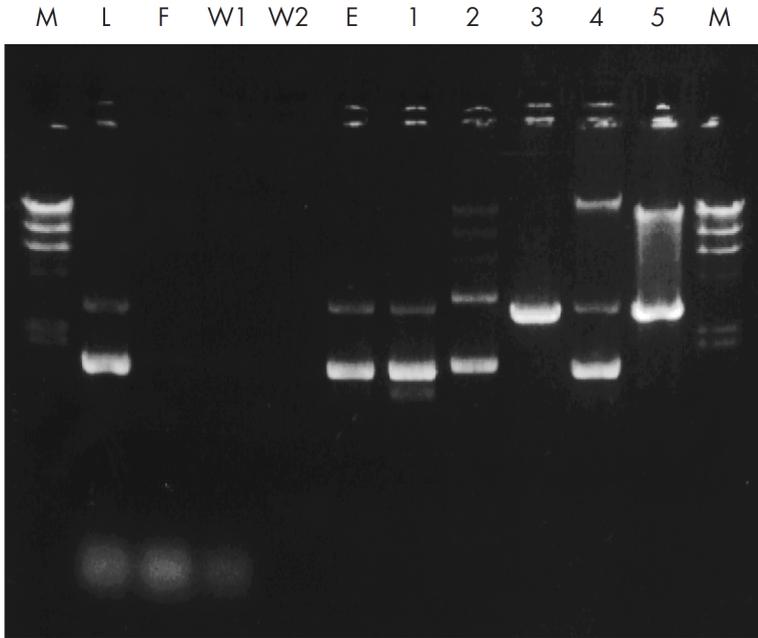


Figure 4. Agarose gel analysis of the plasmid purification procedure.

## Agarose gel analysis

Run 2  $\mu\text{L}$  of each sample on a 1% agarose gel\* for analysis of the fractions at each stage of the plasmid purification procedure. Figure 4 shows an analytical gel of the different fractions, together with examples of problems that can arise at each step. If you find that you have a problem with a particular step of the protocol, turn to the hints in the relevant section of the “Troubleshooting Guide”, page 48. If the problem remains unresolved, or if you have any further questions, please contact QIAGEN Technical Services via [support.qiagen.com](https://support.qiagen.com).

\* When working with chemicals, always wear a suitable lab coat, disposable gloves, and protective goggles. For more information, consult the appropriate safety data sheets (SDSs), available from the product supplier.

- L:** Cleared lysate containing supercoiled and open circular plasmid DNA and degraded RNA (sample 1).
- F:** Flow-through fraction containing only degraded RNA is depleted of plasmid DNA which is bound to the QIAGEN resin (sample 2).
- W1:** First wash fraction, in which the remaining traces of RNA are removed without affecting the binding of the DNA (sample 3).
- W2:** Second wash fraction, which ensures that the resin is completely cleared of RNA and other contaminants, leaving only pure plasmid DNA on the column (sample 3).
- E:** The eluate containing pure plasmid DNA with no other contaminating nucleic acids (sample 4).
- M:** Lambda DNA digested with *HindIII*.\*

Lanes 1–5 illustrate some atypical results that may be observed in some preparations, depending on plasmid type and host strain.

- Lane 1:** Supercoiled (lower band) and open circular form (upper band) of the high-copy plasmid pUC18 with an additional band of denatured supercoiled DNA migrating just below the supercoiled form. This form may result from prolonged alkaline lysis with Buffer P2 and is resistant to restriction digestion.
- Lane 2:** Multimeric forms of supercoiled plasmid DNA (pTZ19) which may be observed with some host strains and should not be mistaken for genomic DNA. Multimeric plasmid DNA can easily be distinguished from genomic DNA by a simple restriction

\* When working with chemicals, always wear a suitable lab coat, disposable gloves, and protective goggles. For more information, consult the appropriate SDSs, available from the product supplier.

digestion–linearization of a plasmid sample displaying multimeric bands will yield a single defined band with the size of the linearized plasmid monomer (see lane 3).

- Lane 3:** Linearized form of plasmid pTZ19 after restriction digestion with *EcoRI*.
- Lane 4:** Sample contaminated with bacterial chromosomal DNA, which may be observed if the lysate is treated too vigorously (e.g., vortexing during incubation steps with Buffer P2 or P3). Genomic DNA contamination can easily be identified by digestion of the sample with *EcoRI*. A smear is observed, in contrast to the linear band seen after digestion of multimeric plasmid forms.
- Lane 5:** *EcoRI* digestion of a sample contaminated with bacterial genomic DNA which gives a smear above the plasmid DNA.

## Appendix B: Composition of Buffers

Buffer	Composition	Storage
Buffer P1 (resuspension buffer)	50 mM Tris-Cl, pH 8.0; 10 mM EDTA; 100 µg/mL RNase A	2–8°C, after addition of RNase A
Buffer P2 (lysis buffer)	200 mM NaOH, 1% SDS (w/v)	15–25°C
Buffer P3 (neutralization buffer)	3.0 M potassium acetate, pH 5.5	15–25°C or 2–8°C
Buffer FWB2 (QIAfilter wash buffer)	1 M potassium acetate pH 5.0	15–25°C
Buffer QBT (equilibration buffer)	750 mM NaCl; 50 mM MOPS, pH 7.0; 15% isopropanol (v/v); 0.15% Triton® X-100 (v/v)	15–25°C
Buffer QC (wash buffer)	1.0 M NaCl; 50 mM MOPS, pH 7.0; 15% isopropanol (v/v)	15–25°C
Buffer QF (elution buffer)	1.25 M NaCl; 50 mM Tris-Cl, pH 8.5; 15% isopropanol (v/v)	15–25°C
Buffer QN (elution buffer)	1.6 M NaCl; 50 mM MOPS, pH 7.0; 15% isopropanol (v/v)	15–25°C
TE	10 mM Tris-Cl, pH 8.0; 1 mM EDTA	15–25°C
STE	100 mM NaCl; 10 mM Tris-Cl, pH 8.0; 1 mM EDTA	15–25°C

## Preparation of buffers

Buffer compositions are given per liter of solution. Do not autoclave MOPS- or isopropanol-containing buffers; sterilize by filtration instead.

Buffer calculations are based on Tris base adjusted to pH with HCl (Tris·Cl). If using Tris·HCl reagent, the quantities used should be recalculated.

- P1: Dissolve 6.06 g Tris base, 3.72 g Na<sub>2</sub>EDTA·2H<sub>2</sub>O in 800 mL distilled water. Adjust the pH to 8.0 with HCl. Adjust the volume to 1 L with distilled water. Add 100 mg RNase A per liter of P1.
- P2: Dissolve 8.0 g NaOH pellets in 950 mL distilled water, 50 mL 20% SDS (w/v) solution. The final volume should be 1 L.
- P3: Dissolve 294.5 g potassium acetate in 500 mL distilled water. Adjust the pH to 5.5 with glacial acetic acid (~110 mL). Adjust the volume to 1 L with distilled water.
- FWB2: Dissolve 98.2 g potassium acetate in 500 mL distilled water. Adjust the pH to 5.0 with glacial acetic acid (~36 mL). Adjust the volume to 1 L with distilled water.
- QBT: Dissolve 43.83 g NaCl, 10.46 g MOPS (free acid), in 800 mL distilled water. Adjust the pH to 7.0 with NaOH. Add 150 mL pure isopropanol and 15 mL 10% Triton X-100 solution (v/v). Adjust the volume to 1 L with distilled water.
- QC: Dissolve 58.44 g NaCl and 10.46 g MOPS (free acid) in 800 mL distilled water. Adjust the pH to 7.0 with NaOH. Add 150 mL pure isopropanol. Adjust the volume to 1 L with distilled water.

- QF: Dissolve 73.05 g NaCl and 6.06 g Tris base in 800 mL distilled water and adjust the pH to 8.5 with HCl. Add 150 mL pure isopropanol. Adjust the volume to 1 L with distilled water.
- QN: Dissolve 93.50 g NaCl and 10.46 g MOPS (free acid) in 800 mL distilled water and adjust the pH to 7.0 with NaOH. Add 150 mL pure isopropanol. Adjust the volume to 1 L with distilled water.
- STE: Dissolve 5.84 g NaCl, 1.21 g Tris base, and 0.37 g Na<sub>2</sub>EDTA·2H<sub>2</sub>O in 800 mL distilled water. Adjust the pH to 8.0 with HCl. Adjust the volume to 1 L with distilled water.

**Note:** Always recheck pH of buffers after preparation.

### Preparation of LB medium

Dissolve 10 g tryptone, 5 g yeast extract, and 10 g NaCl in 800 mL distilled water. Adjust the pH to 7.0 with 1 N NaOH. Adjust the volume to 1 L with distilled water. Sterilize by autoclaving.

# Ordering Information

Product	Contents	Cat. no.
QIAGEN Plasmid Mini Kit (25)	25 QIAGEN-tip 20, reagents, buffers	12123
QIAGEN Plasmid Mini Kit (100)	100 QIAGEN-tip 20, reagents, buffers	12125
QIAGEN Plasmid Midi Kit (25)	25 QIAGEN-tip 100, reagents, buffers	12143
QIAGEN Plasmid Midi Kit (100)	100 QIAGEN-tip 100, reagents, buffers	12145
QIAGEN Plasmid Maxi Kit (10)	10 QIAGEN-tip 500, reagents, buffers	12162
QIAGEN Plasmid Maxi Kit (25)	25 QIAGEN-tip 500, reagents, buffers	12163
QIAGEN Plasmid Maxi Kit (100)	100 QIAGEN-tip 500, reagents, buffers	12165
Plasmid Buffer Set	Buffers P1, P2, P3, QBT, QC, QF, RNase A; for 100 plasmid mini-, 25 midi-, or 10 maxipreps	19046
QIAGEN-tip 20 (25)	25 columns	10023
QIAGEN-tip 100 (25)	25 columns	10043
QIAGEN-tip 500 (25)	25 columns	10063
QIAGEN-tip 2500 (25)	25 columns	10083
QIAGEN-tip 10000 (5)	5 columns	10091

Product	Contents	Cat. no.
<b>QIAGEN Plasmid <i>Plus</i> Kits — for the fastest and most convenient purification of transfection-grade plasmid DNA suitable for all applications</b>		
QIAGEN Plasmid <i>Plus</i> Maxi Kit (25)	25 QIAGEN Plasmid <i>Plus</i> Maxi Columns, extender tubes, reagents, buffers, 25 QIAfilter Maxi Cartridges	12963
QIAGEN Plasmid <i>Plus</i> Midi Kit (25)	25 QIAGEN Plasmid <i>Plus</i> Midi Columns, extender tubes, reagents, buffers, 25 QIAfilter Midi Cartridges	12943
QIAGEN Plasmid <i>Plus</i> Giga Kit (5)	5 QIAGEN Plasmid <i>Plus</i> Mega Columns, extender tubes, reagents, buffers, 5 QIAfilter Mega-Giga Cartridges	12991
QIAGEN Plasmid <i>Plus</i> Mega Kit (5)	5 QIAGEN Plasmid <i>Plus</i> Mega Columns, extender tubes, reagents, buffers, 5 QIAfilter	12981
QIAGEN Plasmid <i>Plus</i> 96 BioRobot Kit (4)	For 4 x 96 plasmid minipreps: TurboFilter 96 Plates and Plasmid <i>Plus</i> 96 Plates, buffers, reagents, flat-bottom blocks, S-Blocks, and elution microtubes; for use with the BioRobot Universal System	960241
<b>QIAfilter Plasmid Kits — for fast purification of transfection-grade plasmid or cosmid DNA</b>		
QIAfilter Plasmid Midi Kit (25)	25 QIAGEN-tip 100, reagents, buffers, 25 QIAfilter Midi Cartridges	12243
QIAfilter Plasmid Maxi Kit (10)	10 QIAGEN-tip 500, reagents, buffers, 10 QIAfilter Maxi Cartridges	12262
QIAfilter Plasmid Mega Kit (5)	5 QIAGEN-tip 2500, reagents, buffers, 5 QIAfilter Mega-Giga Cartridges	12281

Product	Contents	Cat. no.
QIAfilter Plasmid Giga Kit (5)*	5 QIAGEN-tip 10000, reagents, buffers, 5 QIAfilter Mega-Giga Cartridges	12291
QIAfilter Midi Cartridges (25)	25 QIAfilter Midi Cartridges	19743
QIAfilter Maxi Cartridges (25)	25 QIAfilter Maxi Cartridges	19763
QIAfilter Mega-Giga Cartridges (5)	5 QIAfilter Mega-Giga Cartridges, Buffer FWB2	19781
<b>HiSpeed Plasmid Kits — for ultrafast purification of transfection-grade plasmid or cosmid DNA</b>		
HiSpeed Plasmid Midi Kit (25)	25 HiSpeed Midi Tips, 25 QIAfilter Midi Cartridges, 25 QIAprecipitator Midi Modules plus syringes, reagents, buffers	12643
HiSpeed Plasmid Maxi Kit (10)	10 HiSpeed Maxi Tips, 10 QIAfilter Maxi Cartridges, 10 QIAprecipitator Maxi Modules plus syringes, reagents, buffers	12662
HiSpeed Plasmid Maxi Kit (25)	25 HiSpeed Maxi Tips, 25 QIAfilter Maxi Cartridges, 25 QIAprecipitator Maxi Modules plus syringes, reagents, buffers	12663
<b>EndoFree Plasmid Kits — for purification of endotoxin-free advanced transfection-grade plasmid or cosmid DNA</b>		
EndoFree Plasmid Maxi Kit (10)	10 QIAGEN-tip 500, reagents, 10 QIAfilter Maxi Cartridges, endotoxin-free buffers	12362

\* For purification of low-copy plasmids and cosmids, QIAfilter Plasmid Mega Kits are a better choice than QIAfilter Plasmid Giga Kits, due to the large culture volumes required and the limited capacity of the QIAfilter Mega-Giga Cartridge.

Product	Contents	Cat. no.
EndoFree Plasmid Mega Kit (5)	5 QIAGEN-tip 2500, reagents, 5 QIAfilter Mega-Giga Cartridges, endotoxin-free buffers	12381
EndoFree Plasmid Giga Kit (5)*	5 QIAGEN-tip 10000, reagents, 5 QIAfilter Mega-Giga Cartridges, endotoxin-free buffers	12391
<b>QIAprep® Spin Kit — for purification of molecular biology grade plasmid DNA</b>		
QIAprep Spin Miniprep Kit (50)	50 QIAprep Spin Columns, 27104 reagents, buffers, collection tubes (2 mL)	27104
<b>CompactPrep® Plasmid Kits* — for fast purification of molecular biology grade plasmid DNA</b>		
CompactPrep Plasmid Midi Kit (25)	25 CompactPrep Midi Columns, extender tubes, reagents, buffers, LyseBlue	12843
CompactPrep Plasmid Maxi Kit (25)	25 CompactPrep Maxi Columns, extender tubes, reagents, buffers, LyseBlue	12863
<b>QIAGEN Large-Construct Kit — for purification of BAC, PAC, and P1 DNA or up to 200 µg cosmid DNA, free of genomic DNA</b>		
QIAGEN Large-Construct Kit (10)	10 QIAGEN-tip 500, reagents, buffers, ATP-dependent exonuclease†	12462
<b>Transfection products</b>		
PolyFect Transfection Reagent (1 mL)	For 25–65 transfections in 60 mm dishes or 50–100 transfections in 6-well plates	301105
Effectene Transfection Reagent (1 mL)	For 40 transfections in 60 mm dishes or 160 transfections in 12-well plates	301425

\* CompactPrep Kits require use of a vacuum device for operation (e.g., QIAvac 24 Plus, cat. no. 19413).

† ATP solution for exonuclease digestion is not provided.

Product	Contents	Cat. no.
SuperFect Transfection Reagent (1.2 mL)	For 40 transfections in 60 mm dishes or 160 transfections in 12-well plates	301305
<b>Accessories</b>		
QIAvac 24 Plus	Vacuum manifold for processing 1–24 spin columns: QIAvac 24 Plus Vacuum manifold, luer plugs, quick couplings	19413
QIARack	1 rack for 12 x QIAGEN-tip 20, 8 x QIAGEN-tip 100, 6 x QIAGEN-tip 500 or HiSpeed Midi Tips, 4 x QIAGEN-tip 2500 or HiSpeed Maxi Tips, and 10 QIAfilter Midi or Maxi Cartridges	19015
RNase A (17,500 U)	2.5 mL (100 mg/mL; 7000 units/mL solution)	19101
Plasmid Buffer Set	Buffers P1, P2, P3, QBT, QC, QF, RNase A; for 100 plasmid minipreps, 25 midipreps, or 10 maxipreps	19046
EndoFree Plasmid Buffer Set	Buffers P1, P2, P3, QBT, QC, QN, ER, TE, endotoxin-free water, RNase A; for 10 plasmid megapreps or 5 gigapreps (endotoxin-free)	19048
Buffer P1	500 mL Resuspension Buffer (RNase A not included)	19051
Buffer P2	500 mL Lysis Buffer	19052
Buffer P3	500 mL Neutralization Buffer	19053

For up-to-date licensing information and product-specific disclaimers, see the respective QIAGEN kit handbook or user manual. QIAGEN kit handbooks and user manuals are available at [www.qiagen.com](http://www.qiagen.com) or can be requested from QIAGEN Technical Services or your local distributor.

# Document Revision History

Date	Changes
02/2021	Added a figure for QIAfilter Mega-Giga Cartridge, the QIAfilter protocol, troubleshooting guide regarding QIAfilter, and “QIAfilter Midi Cartridges”, “QIAfilter Maxi Cartridges”, and “QIAfilter Mega-Giga Cartridges” to the Ordering Information section. Removed “QIAGEN Plasmid Mega Kits” and “QIAGEN Plasmid Giga Kit” from the Ordering Information section.
07/2023	Specified centrifugation temperature in steps 7 and 12 under “Protocol: Plasmid or Cosmid DNA Purification Using QIAGEN Plasmid Mini Kit”.

#### Limited License Agreement for the QIAGEN Plasmid Purification Kit

Use of this product signifies the agreement of any purchaser or user of the product to the following terms:

1. The product may be used solely in accordance with the protocols provided with the product and this handbook and for use with components contained in the kit only. QIAGEN grants no license under any of its intellectual property to use or incorporate the enclosed components of this kit with any components not included within this kit except as described in the protocols provided with the product, this handbook, and additional protocols available at [www.qiagen.com](http://www.qiagen.com). Some of these additional protocols have been provided by QIAGEN users for QIAGEN users. These protocols have not been thoroughly tested or optimized by QIAGEN. QIAGEN neither guarantees them nor warrants that they do not infringe the rights of third-parties.
2. Other than expressly stated licenses, QIAGEN makes no warranty that this kit and/or its use(s) do not infringe the rights of third-parties.
3. This kit and its components are licensed for one-time use and may not be reused, refurbished, or resold.
4. QIAGEN specifically disclaims any other licenses, expressed or implied other than those expressly stated.
5. The purchaser and user of the kit agree not to take or permit anyone else to take any steps that could lead to or facilitate any acts prohibited above. QIAGEN may enforce the prohibitions of this Limited License Agreement in any Court, and shall recover all its investigative and Court costs, including attorney fees, in any action to enforce this Limited License Agreement or any of its intellectual property rights relating to the kit and/or its components.

For updated license terms, see [www.qiagen.com](http://www.qiagen.com).

Trademarks: QIAGEN®, Sample to Insight®, QIAprep®, CompactPrep®, Effectene®, EndoFree®, HiSpeed®, LyseBlue®, PolyFect®, SuperFect® (QIAGEN Group); DH5® (Thermo Fisher Scientific or its subsidiaries); pBluescript® (Agilent Technologies, Inc.); pGEM® (Promega Corporation), Triton® (Union Carbide Corporation). Registered names, trademarks, etc. used in this document, even when not specifically marked as such, are not to be considered unprotected by law.

07/2023 HB-1193-006 © 2023 QIAGEN, all rights reserved.

